

US010449035B2

(12) **United States Patent**
Elahi

(10) **Patent No.:** **US 10,449,035 B2**
(45) **Date of Patent:** **Oct. 22, 2019**

(54) **EXPANDABLE SURGICAL IMPLANT DEVICE**

(71) Applicant: **Ebrahim Elahi**, New York, NY (US)

(72) Inventor: **Ebrahim Elahi**, New York, NY (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 754 days.

(21) Appl. No.: **15/157,248**

(22) Filed: **May 17, 2016**

(65) **Prior Publication Data**

US 2016/0256206 A1 Sep. 8, 2016

Related U.S. Application Data

(63) Continuation of application No. 13/959,539, filed on Aug. 5, 2013, now abandoned.

(51) **Int. Cl.**

- A61F 2/14* (2006.01)
- A61F 2/28* (2006.01)
- A61F 2/00* (2006.01)
- A61F 9/00* (2006.01)
- A61B 17/00* (2006.01)
- A61B 17/80* (2006.01)
- A61F 9/007* (2006.01)

(52) **U.S. Cl.**

CPC *A61F 2/14* (2013.01); *A61B 17/00234* (2013.01); *A61B 17/8061* (2013.01); *A61F 2/0059* (2013.01); *A61F 2/2846* (2013.01); *A61F 9/007* (2013.01); *A61F 9/0017* (2013.01); *A61B 17/8085* (2013.01); *A61B 2017/00946* (2013.01); *A61F 2002/2878* (2013.01); *A61F 2220/0025* (2013.01); *A61F 2250/0024* (2013.01)

(58) **Field of Classification Search**

CPC . *A61B 17/56*; *A61B 17/8023*; *A61B 17/0057*;

A61B 2017/00588; *A61B 2017/0061*;
A61B 2017/00619; *A61F 2/14*; *A61F 2250/0006*; *A61F 2002/2878*; *A61F 2/0059*; *A61F 2/284*; *A61F 9/00176*;
A61F 9/007

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,296,501 A *	10/1981	Kelman	<i>A61F 2/16</i> 623/6.43
9,370,415 B2 *	6/2016	Elahi	<i>A61F 2/0059</i>
2004/0102776 A1 *	5/2004	Huebner	<i>A61B 17/1728</i> 606/281
2006/0116682 A1 *	6/2006	Longo	<i>A61B 17/8061</i> 606/280
2006/0229610 A1 *	10/2006	Piehl	<i>A61B 17/7055</i> 606/71
2010/0292801 A1 *	11/2010	Hansell	<i>A61F 2/442</i> 623/17.16


* cited by examiner

Primary Examiner — William H Matthews

(57) **ABSTRACT**

A surgical implant device may include a first substantially planar portion having a first surface area, a second substantially planar portion having a second surface area, and a coupling device for connecting the first substantially planar portion to the second substantially planar portion. The coupling device facilitates expanding and contracting the first and the second substantially planar portion in order to provide an implant surface area corresponding to the first surface area during insertion of the surgical implant within an incision, and having a third surface area corresponding to both the first surface area and at least a portion of the second surface area following insertion of the surgical implant within the incision.

4 Claims, 8 Drawing Sheets

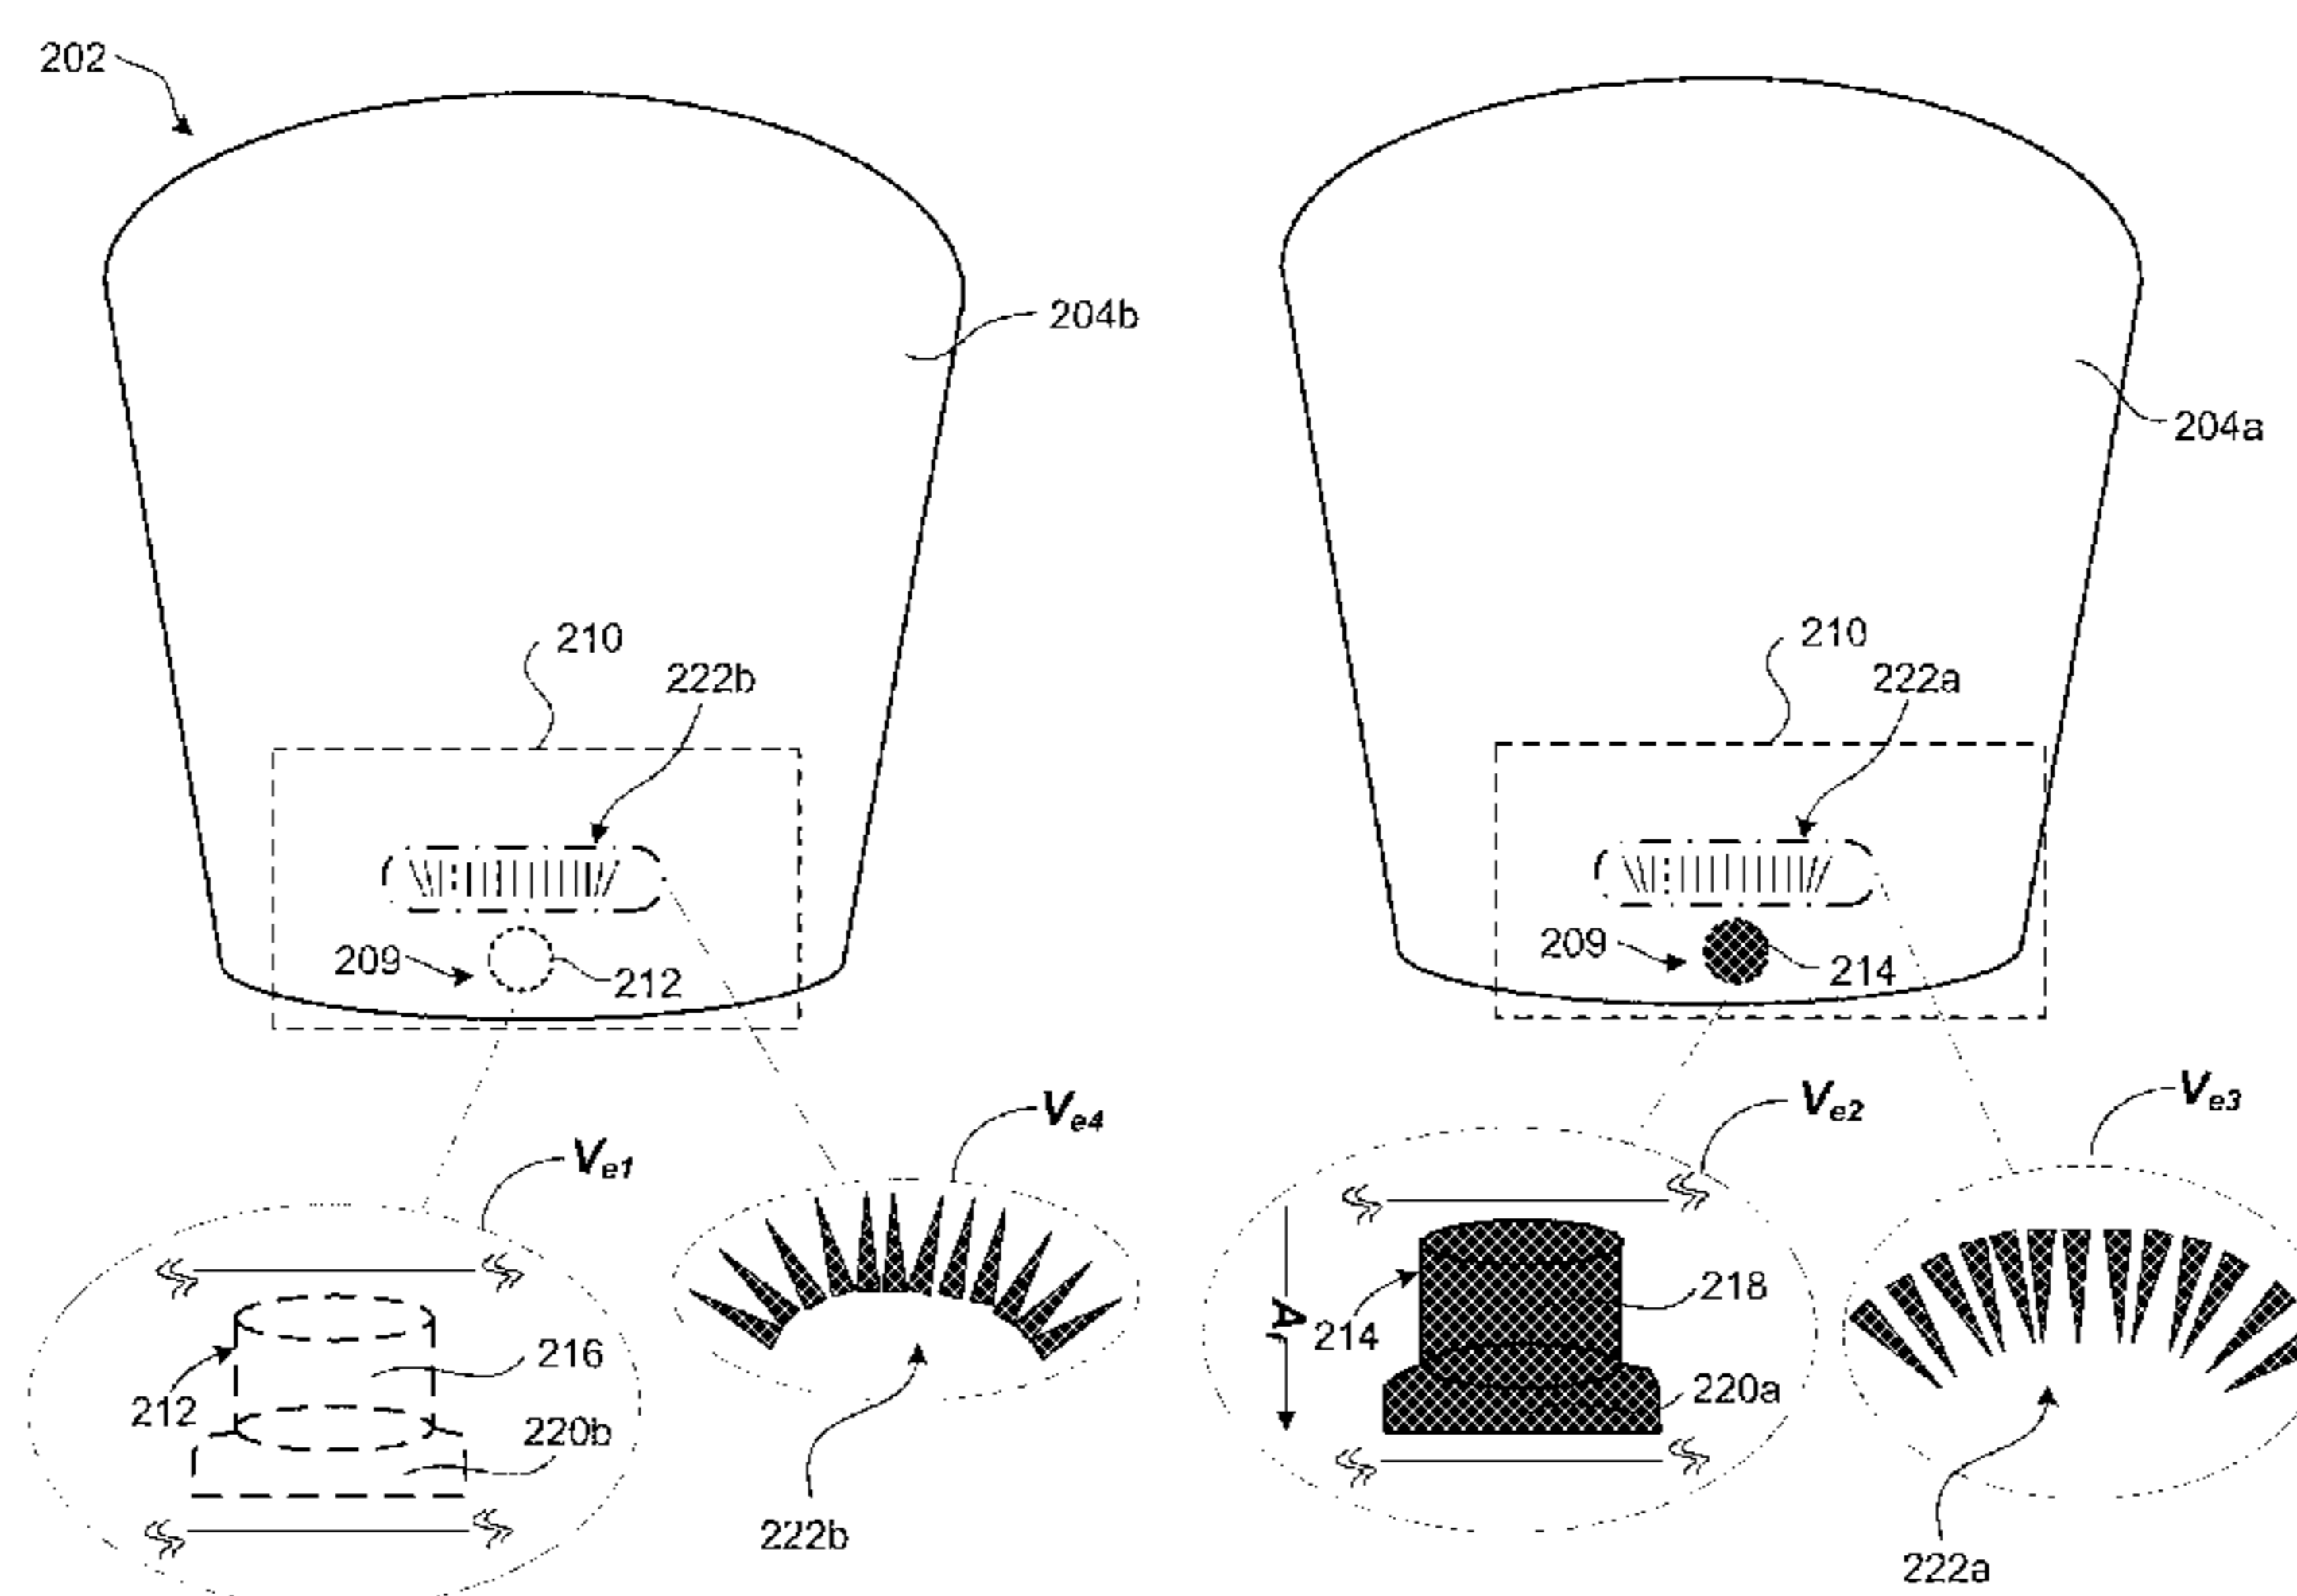

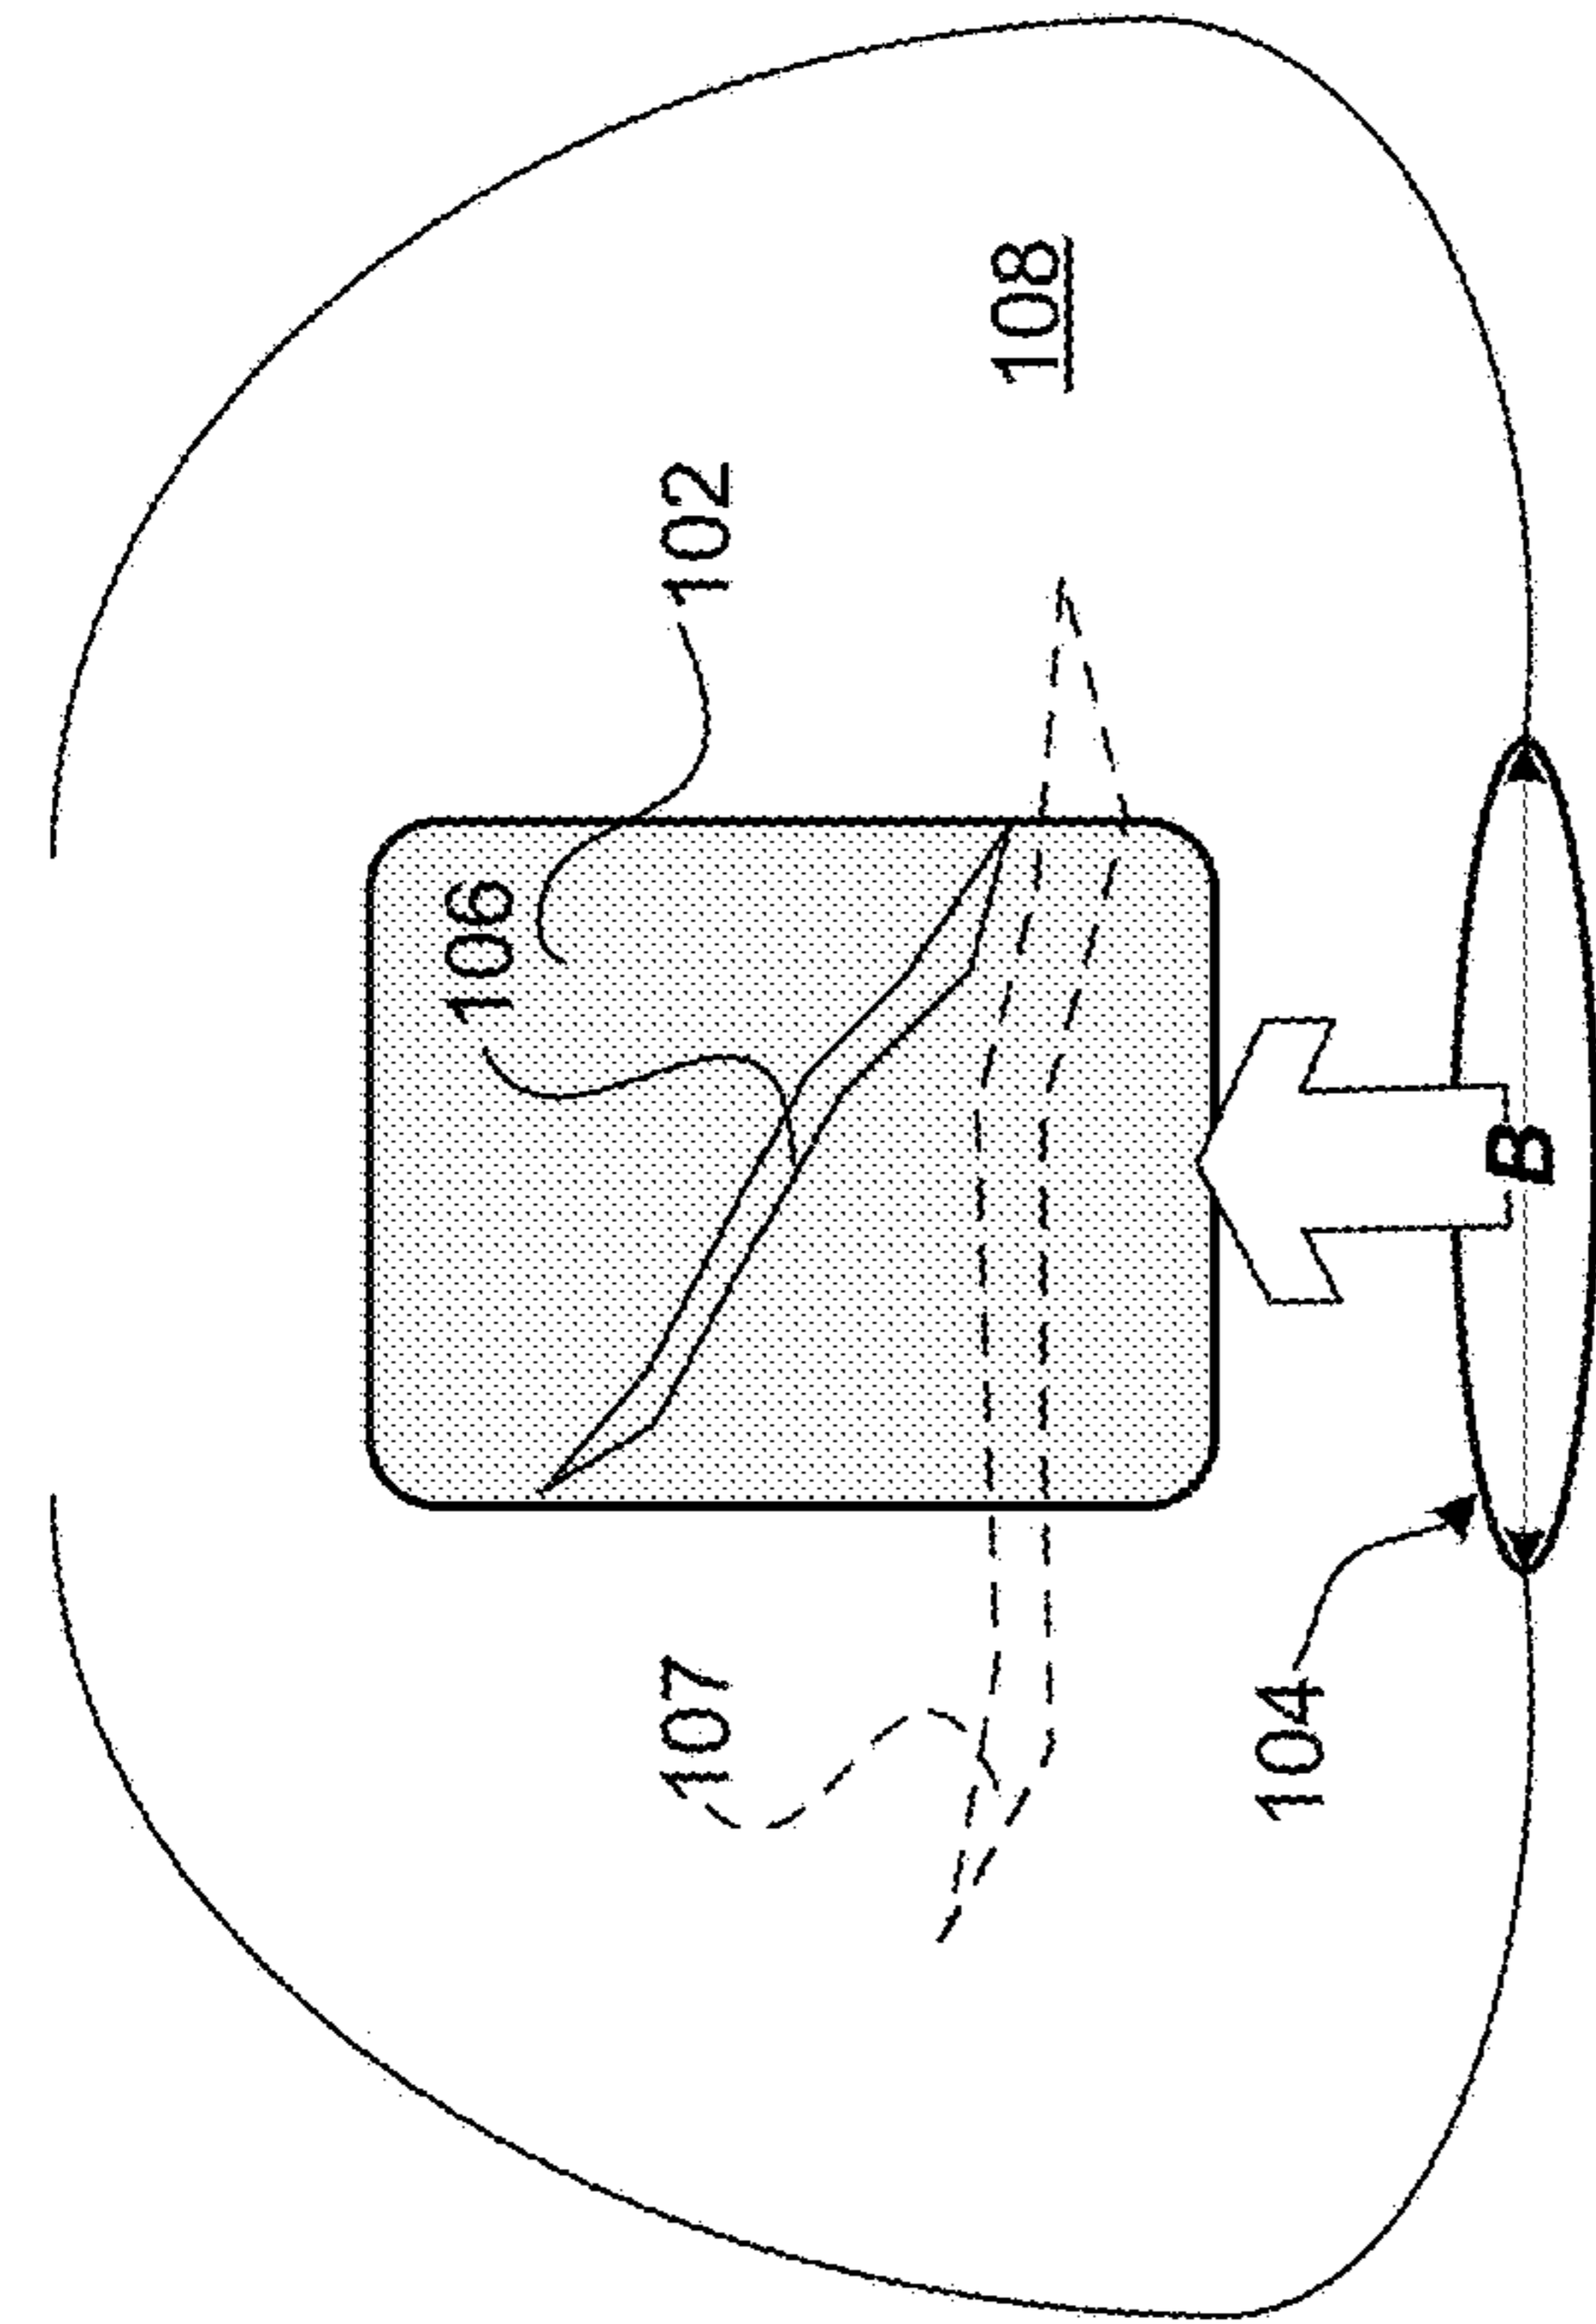


FIG. 1A

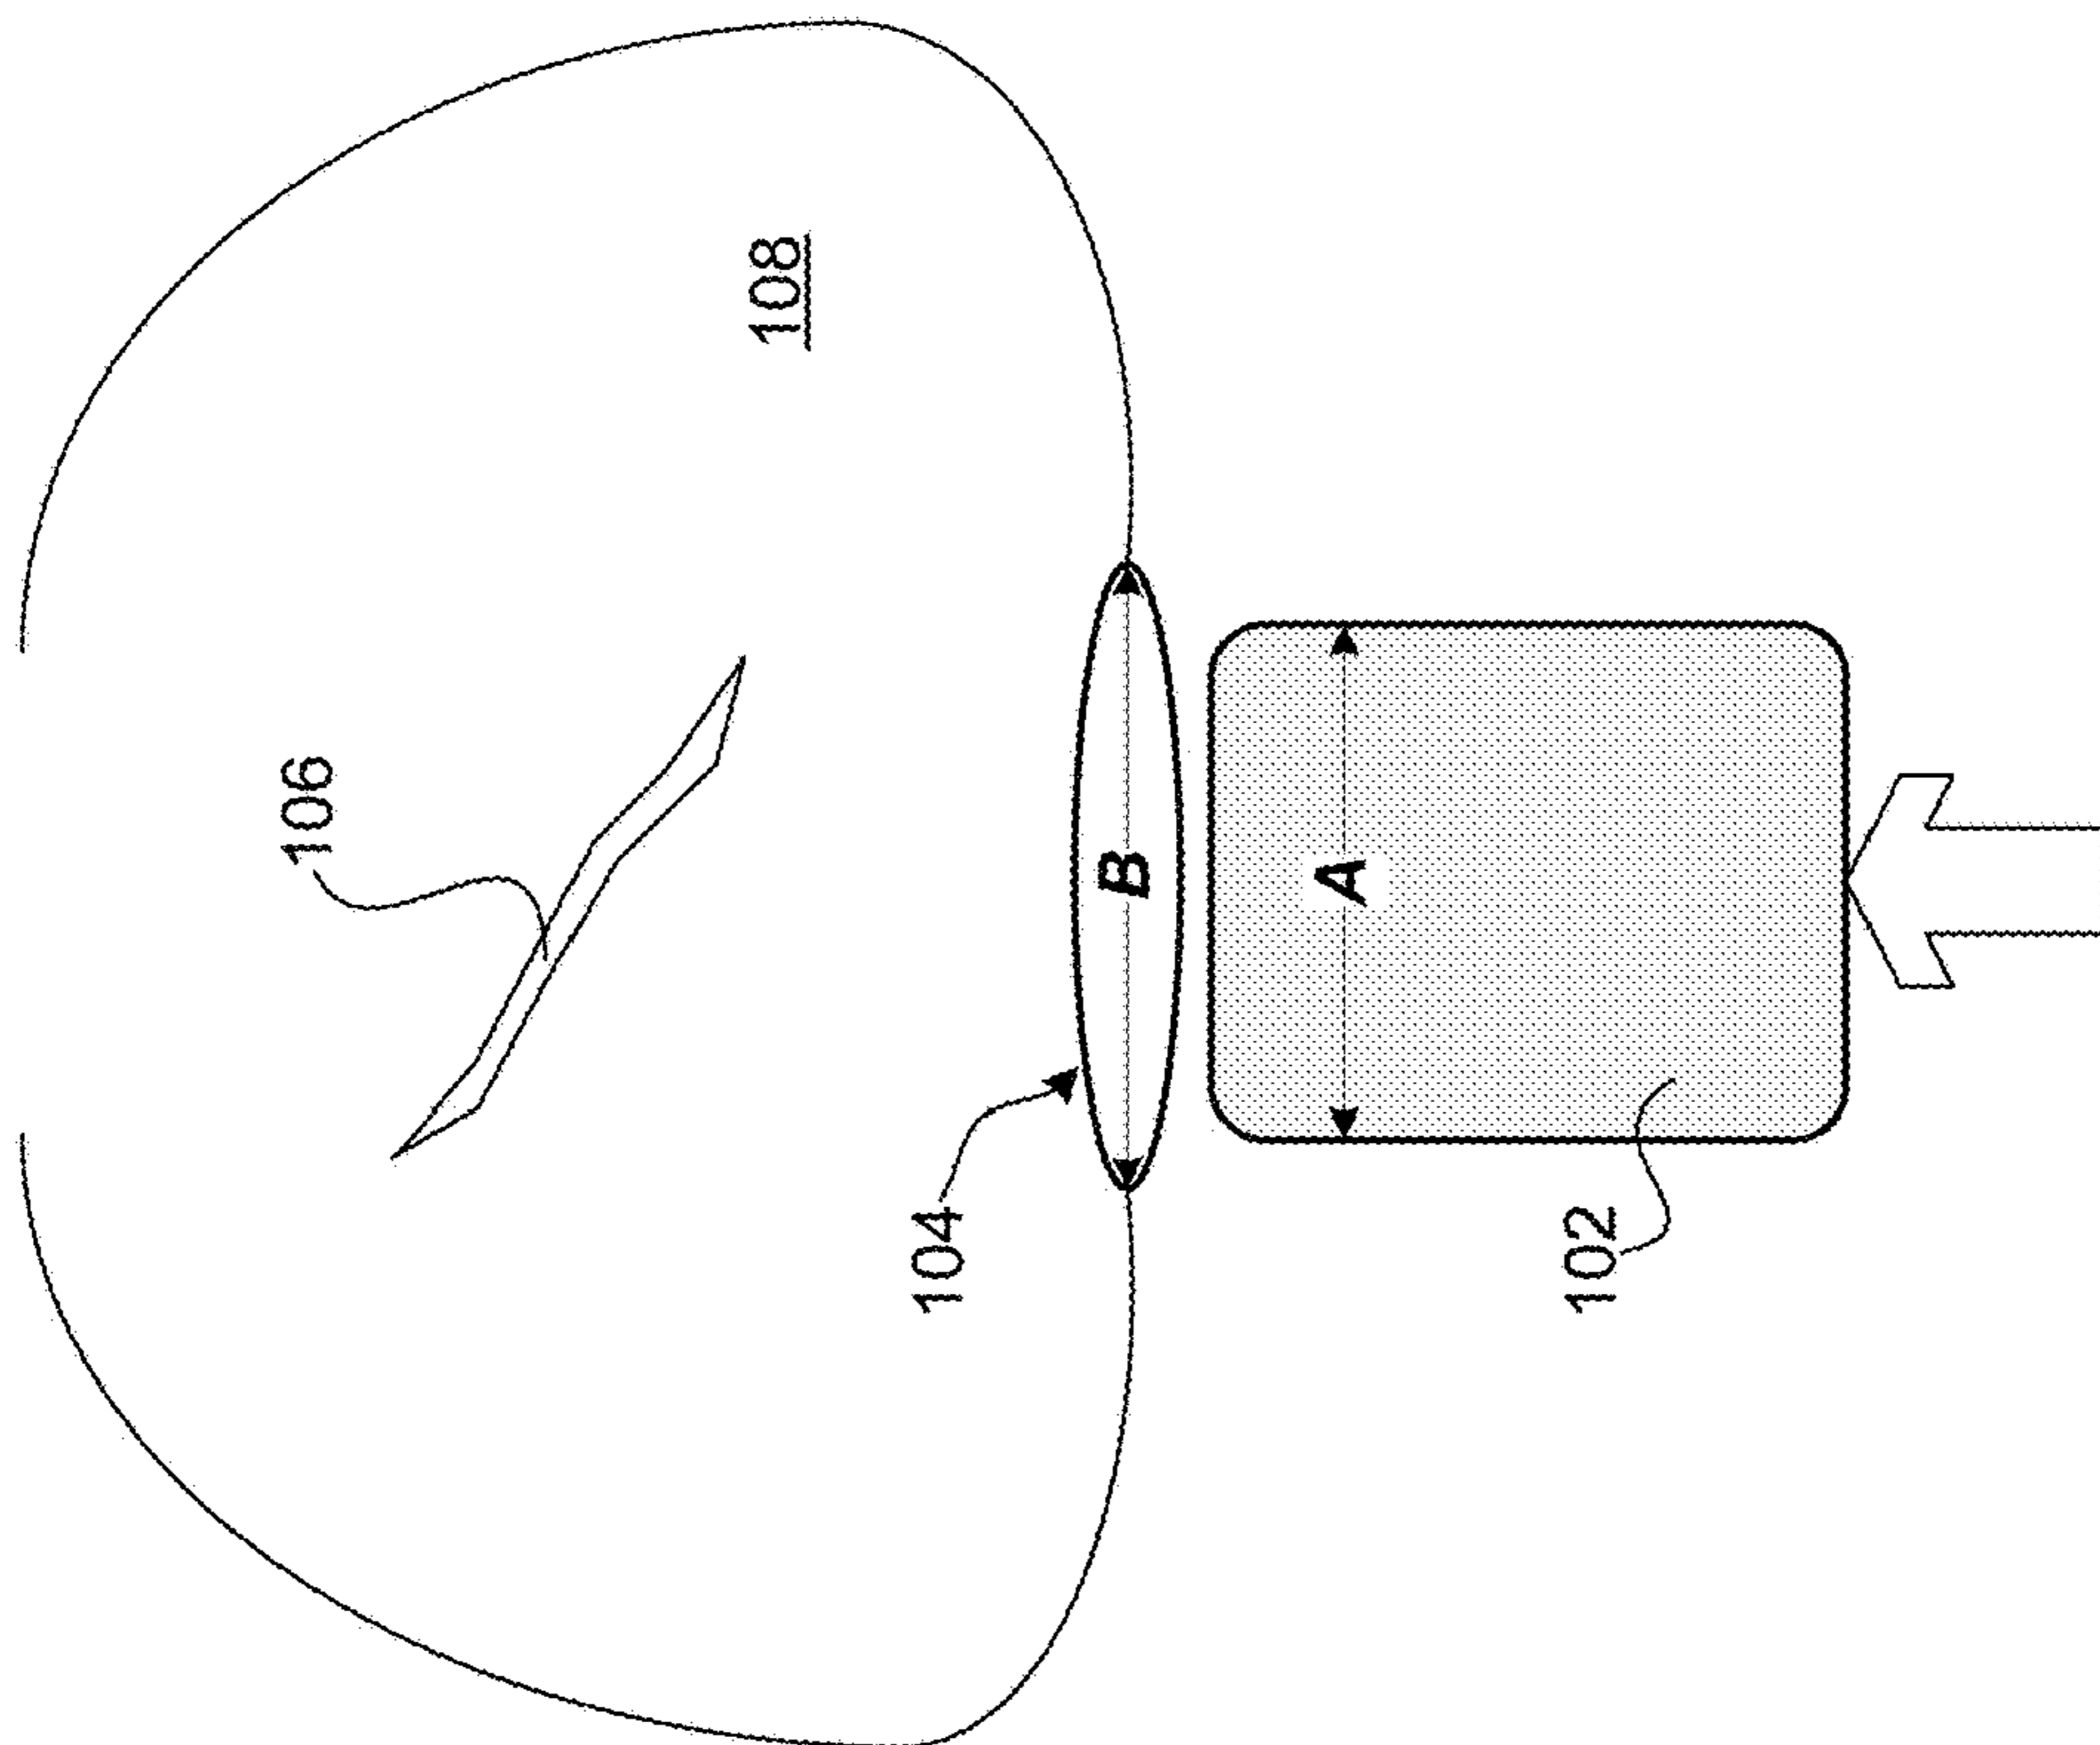


FIG. 1B

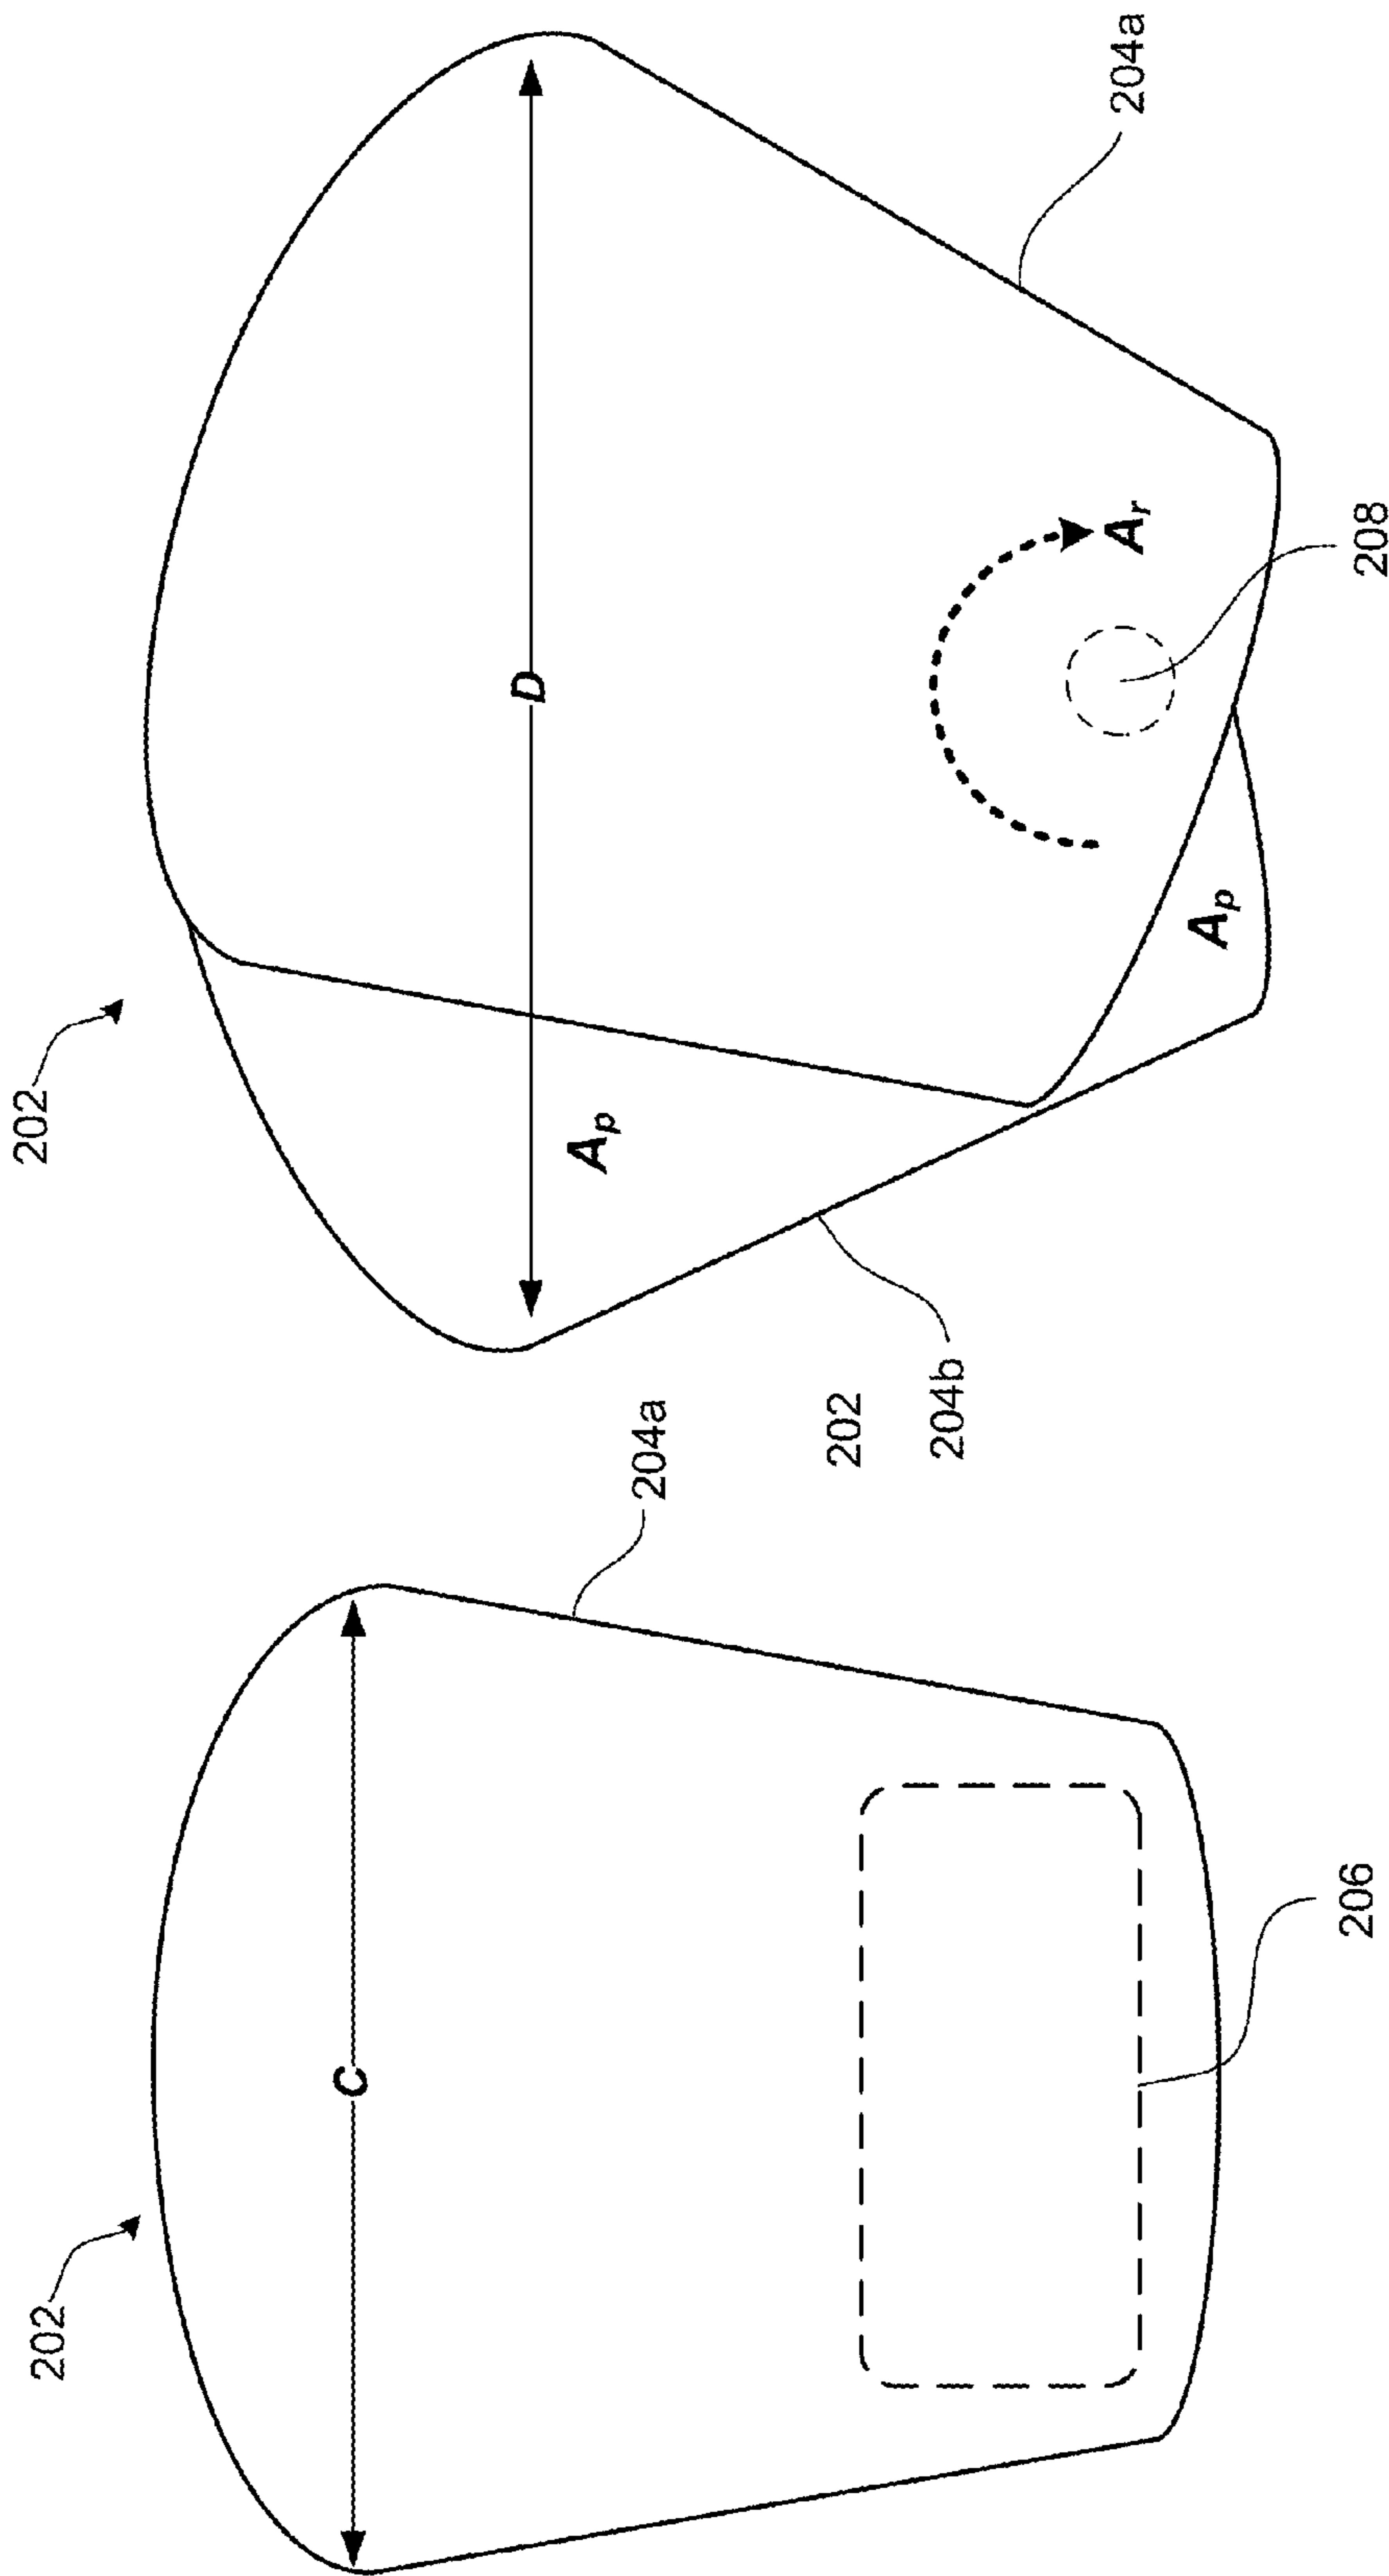


FIG. 2B

FIG. 2A

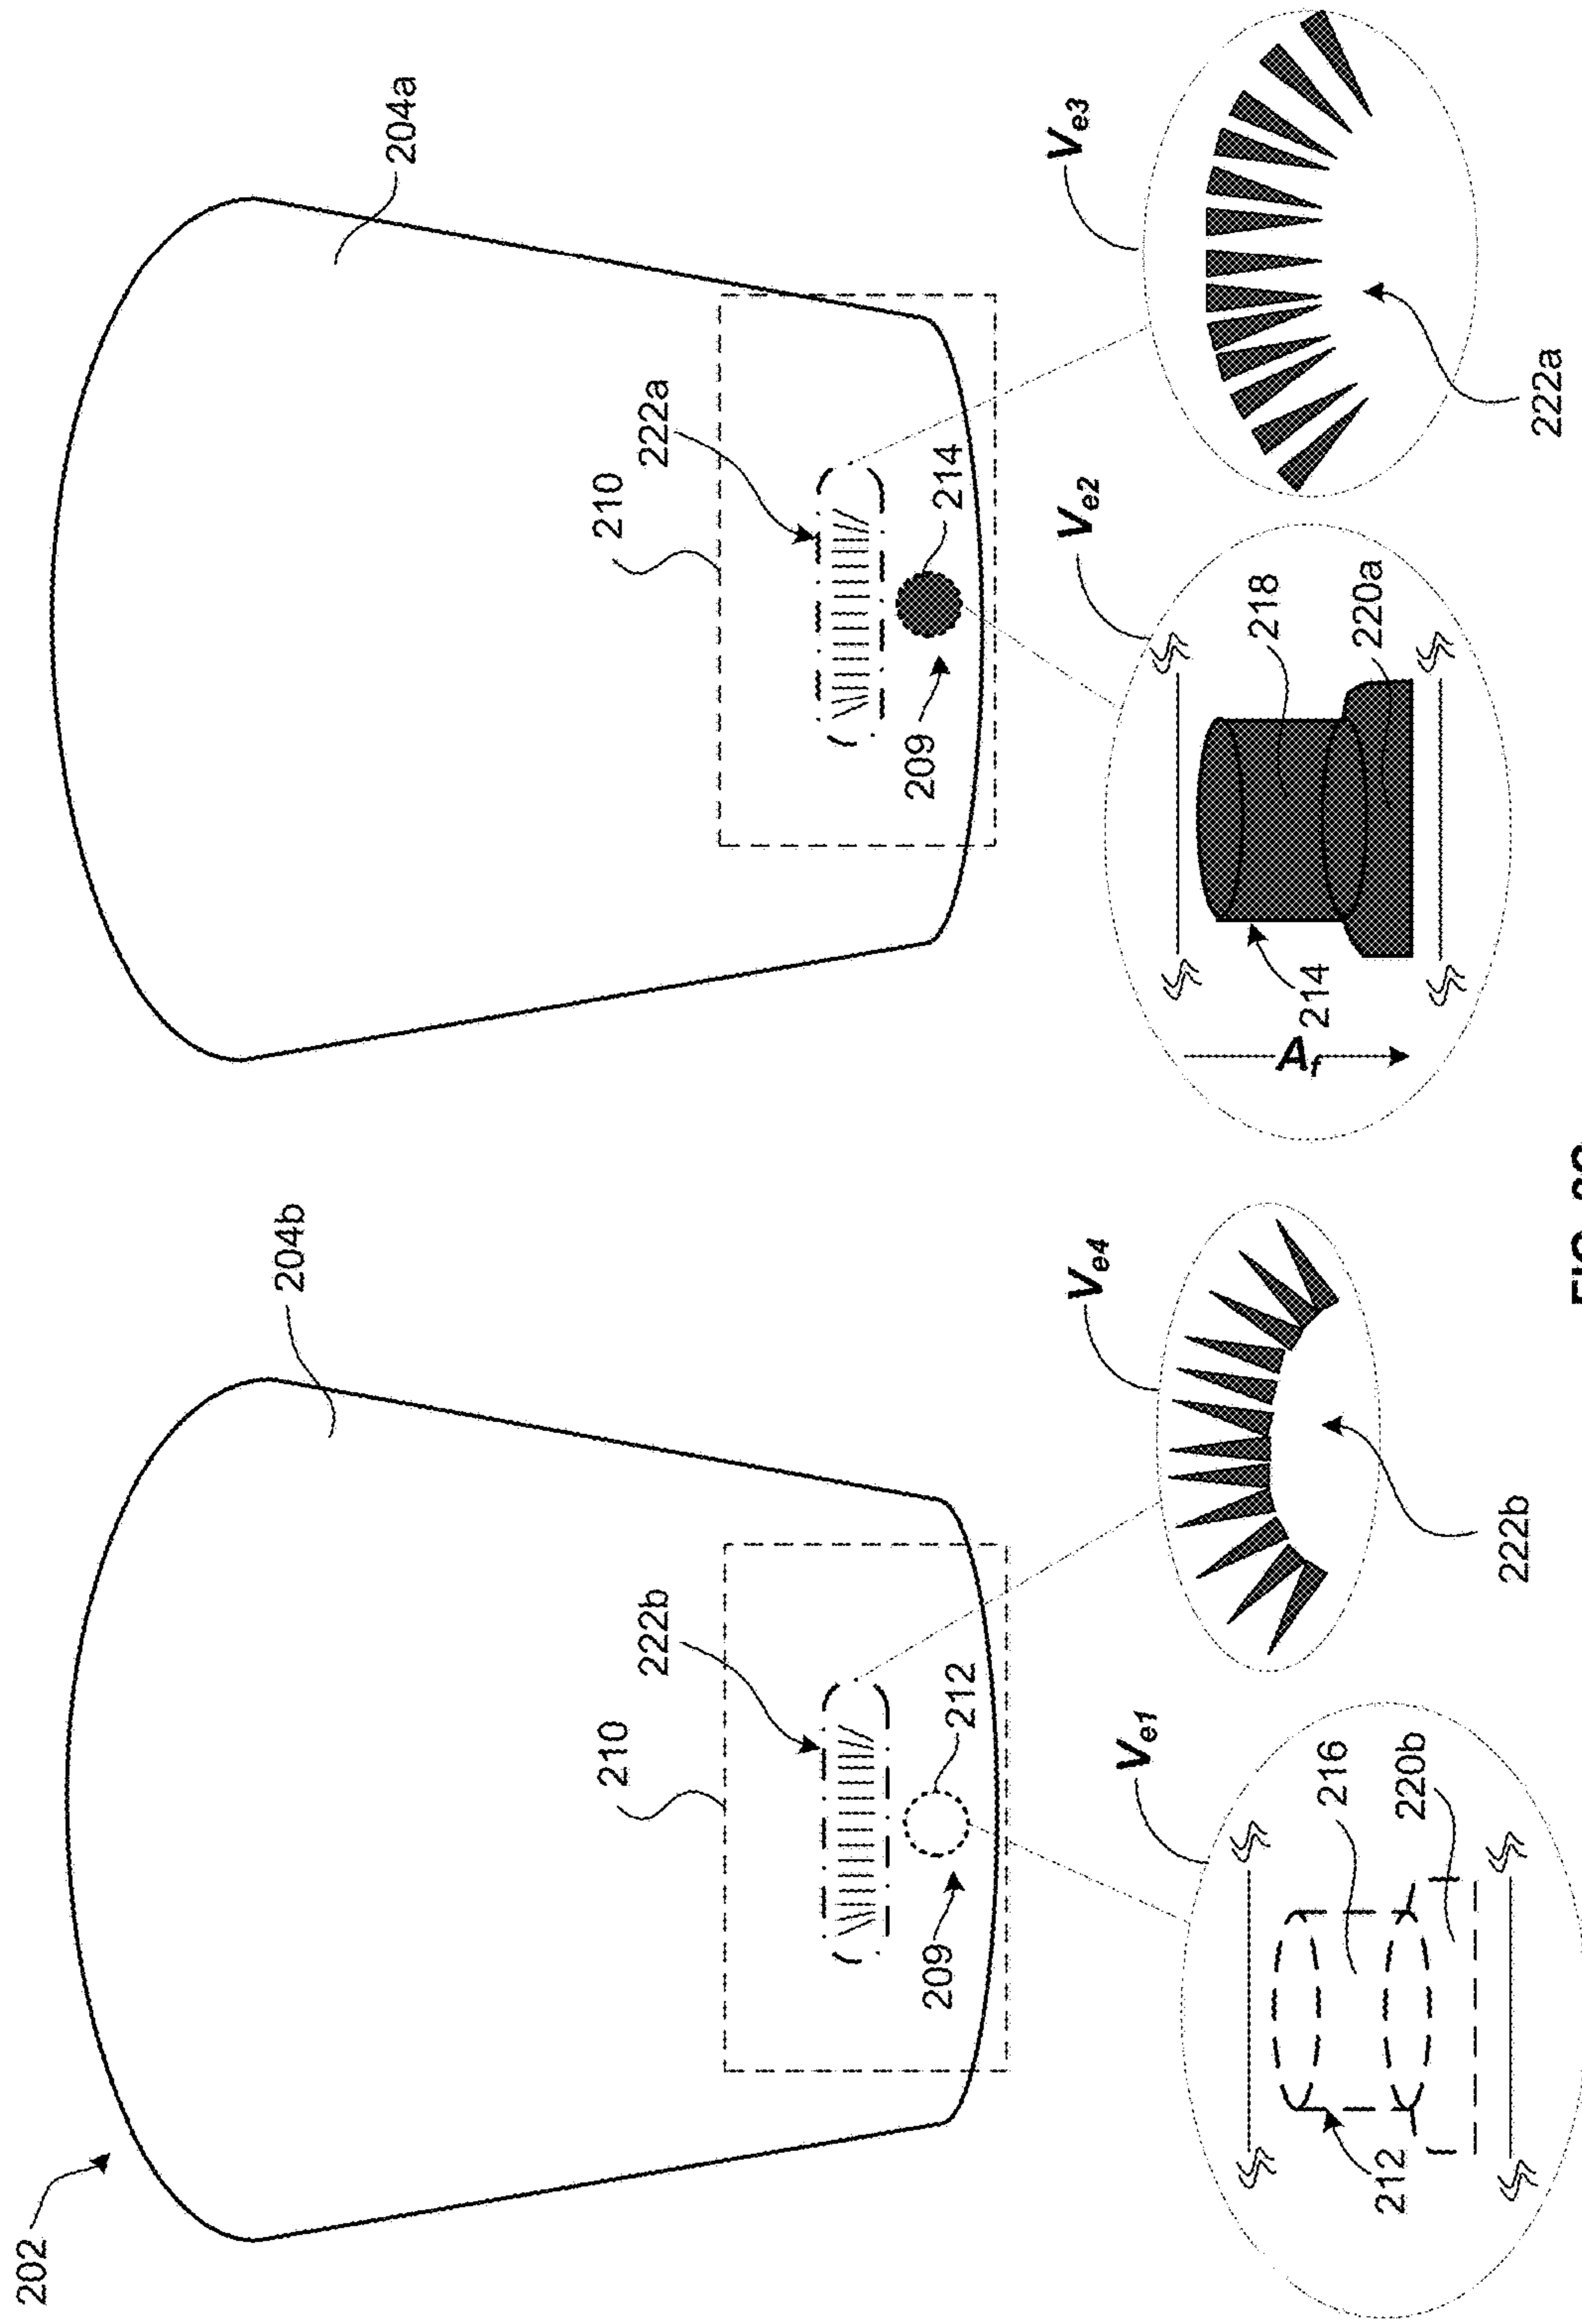


FIG. 2C

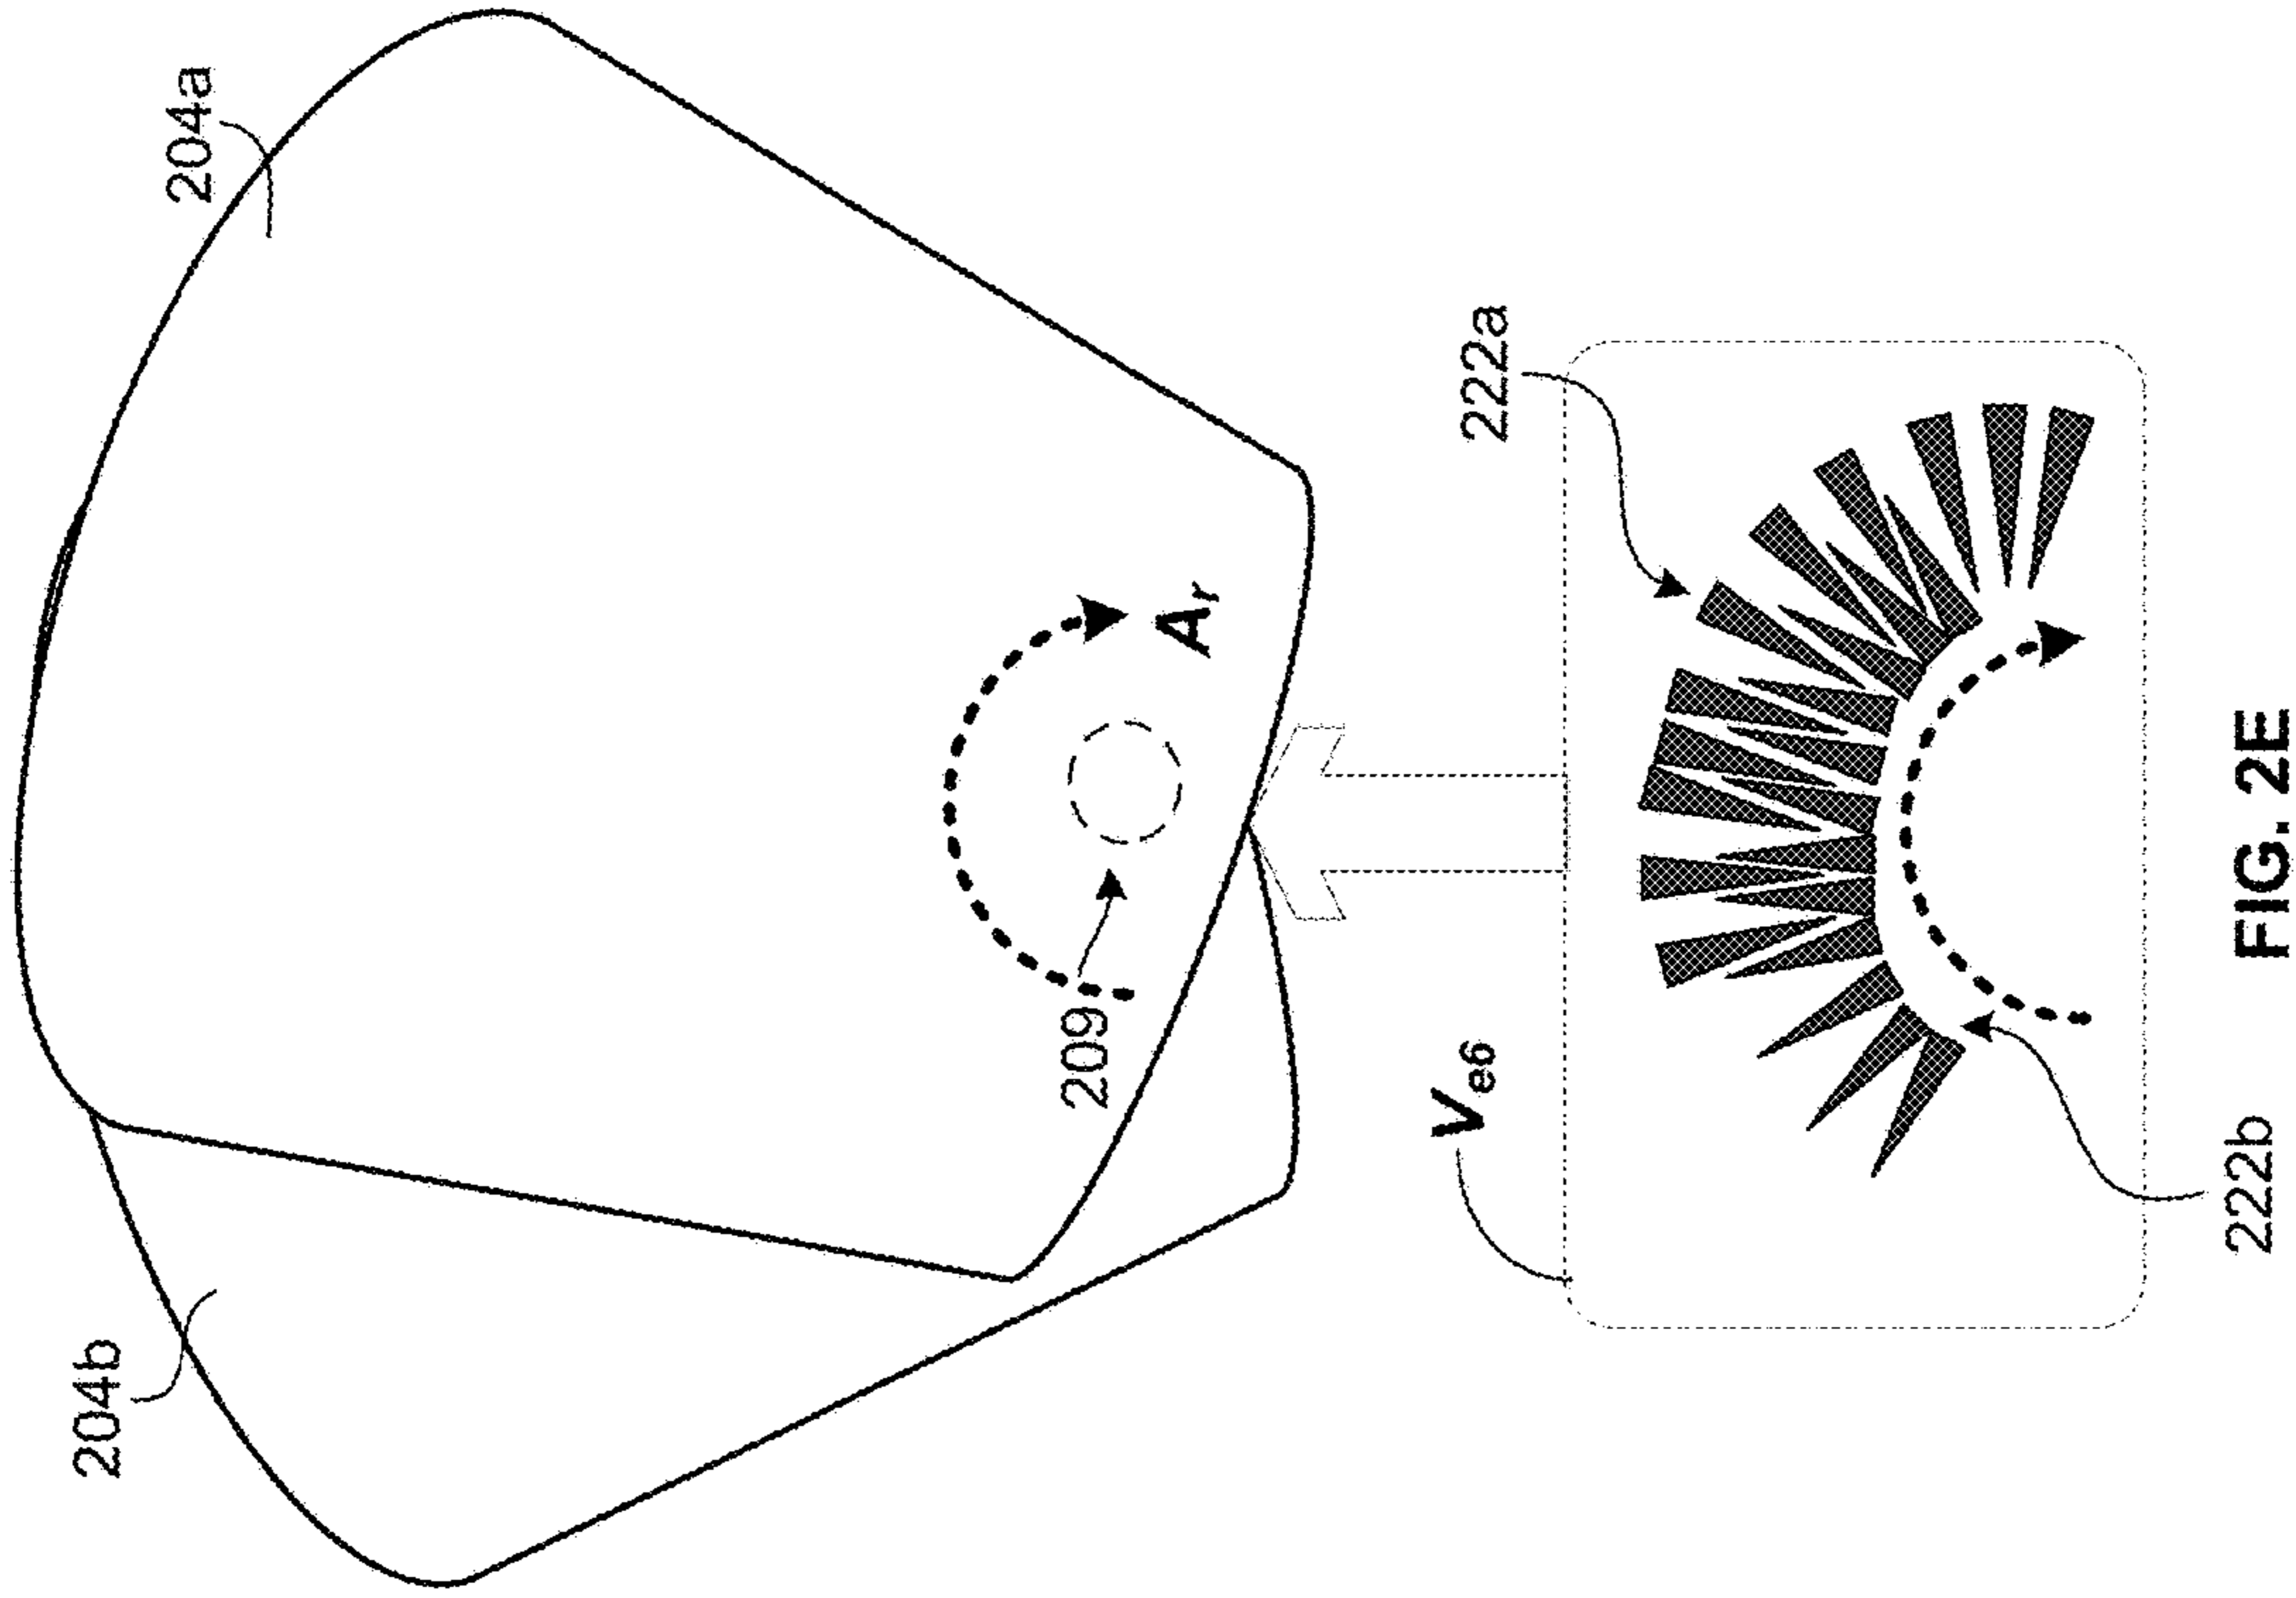


FIG. 2E

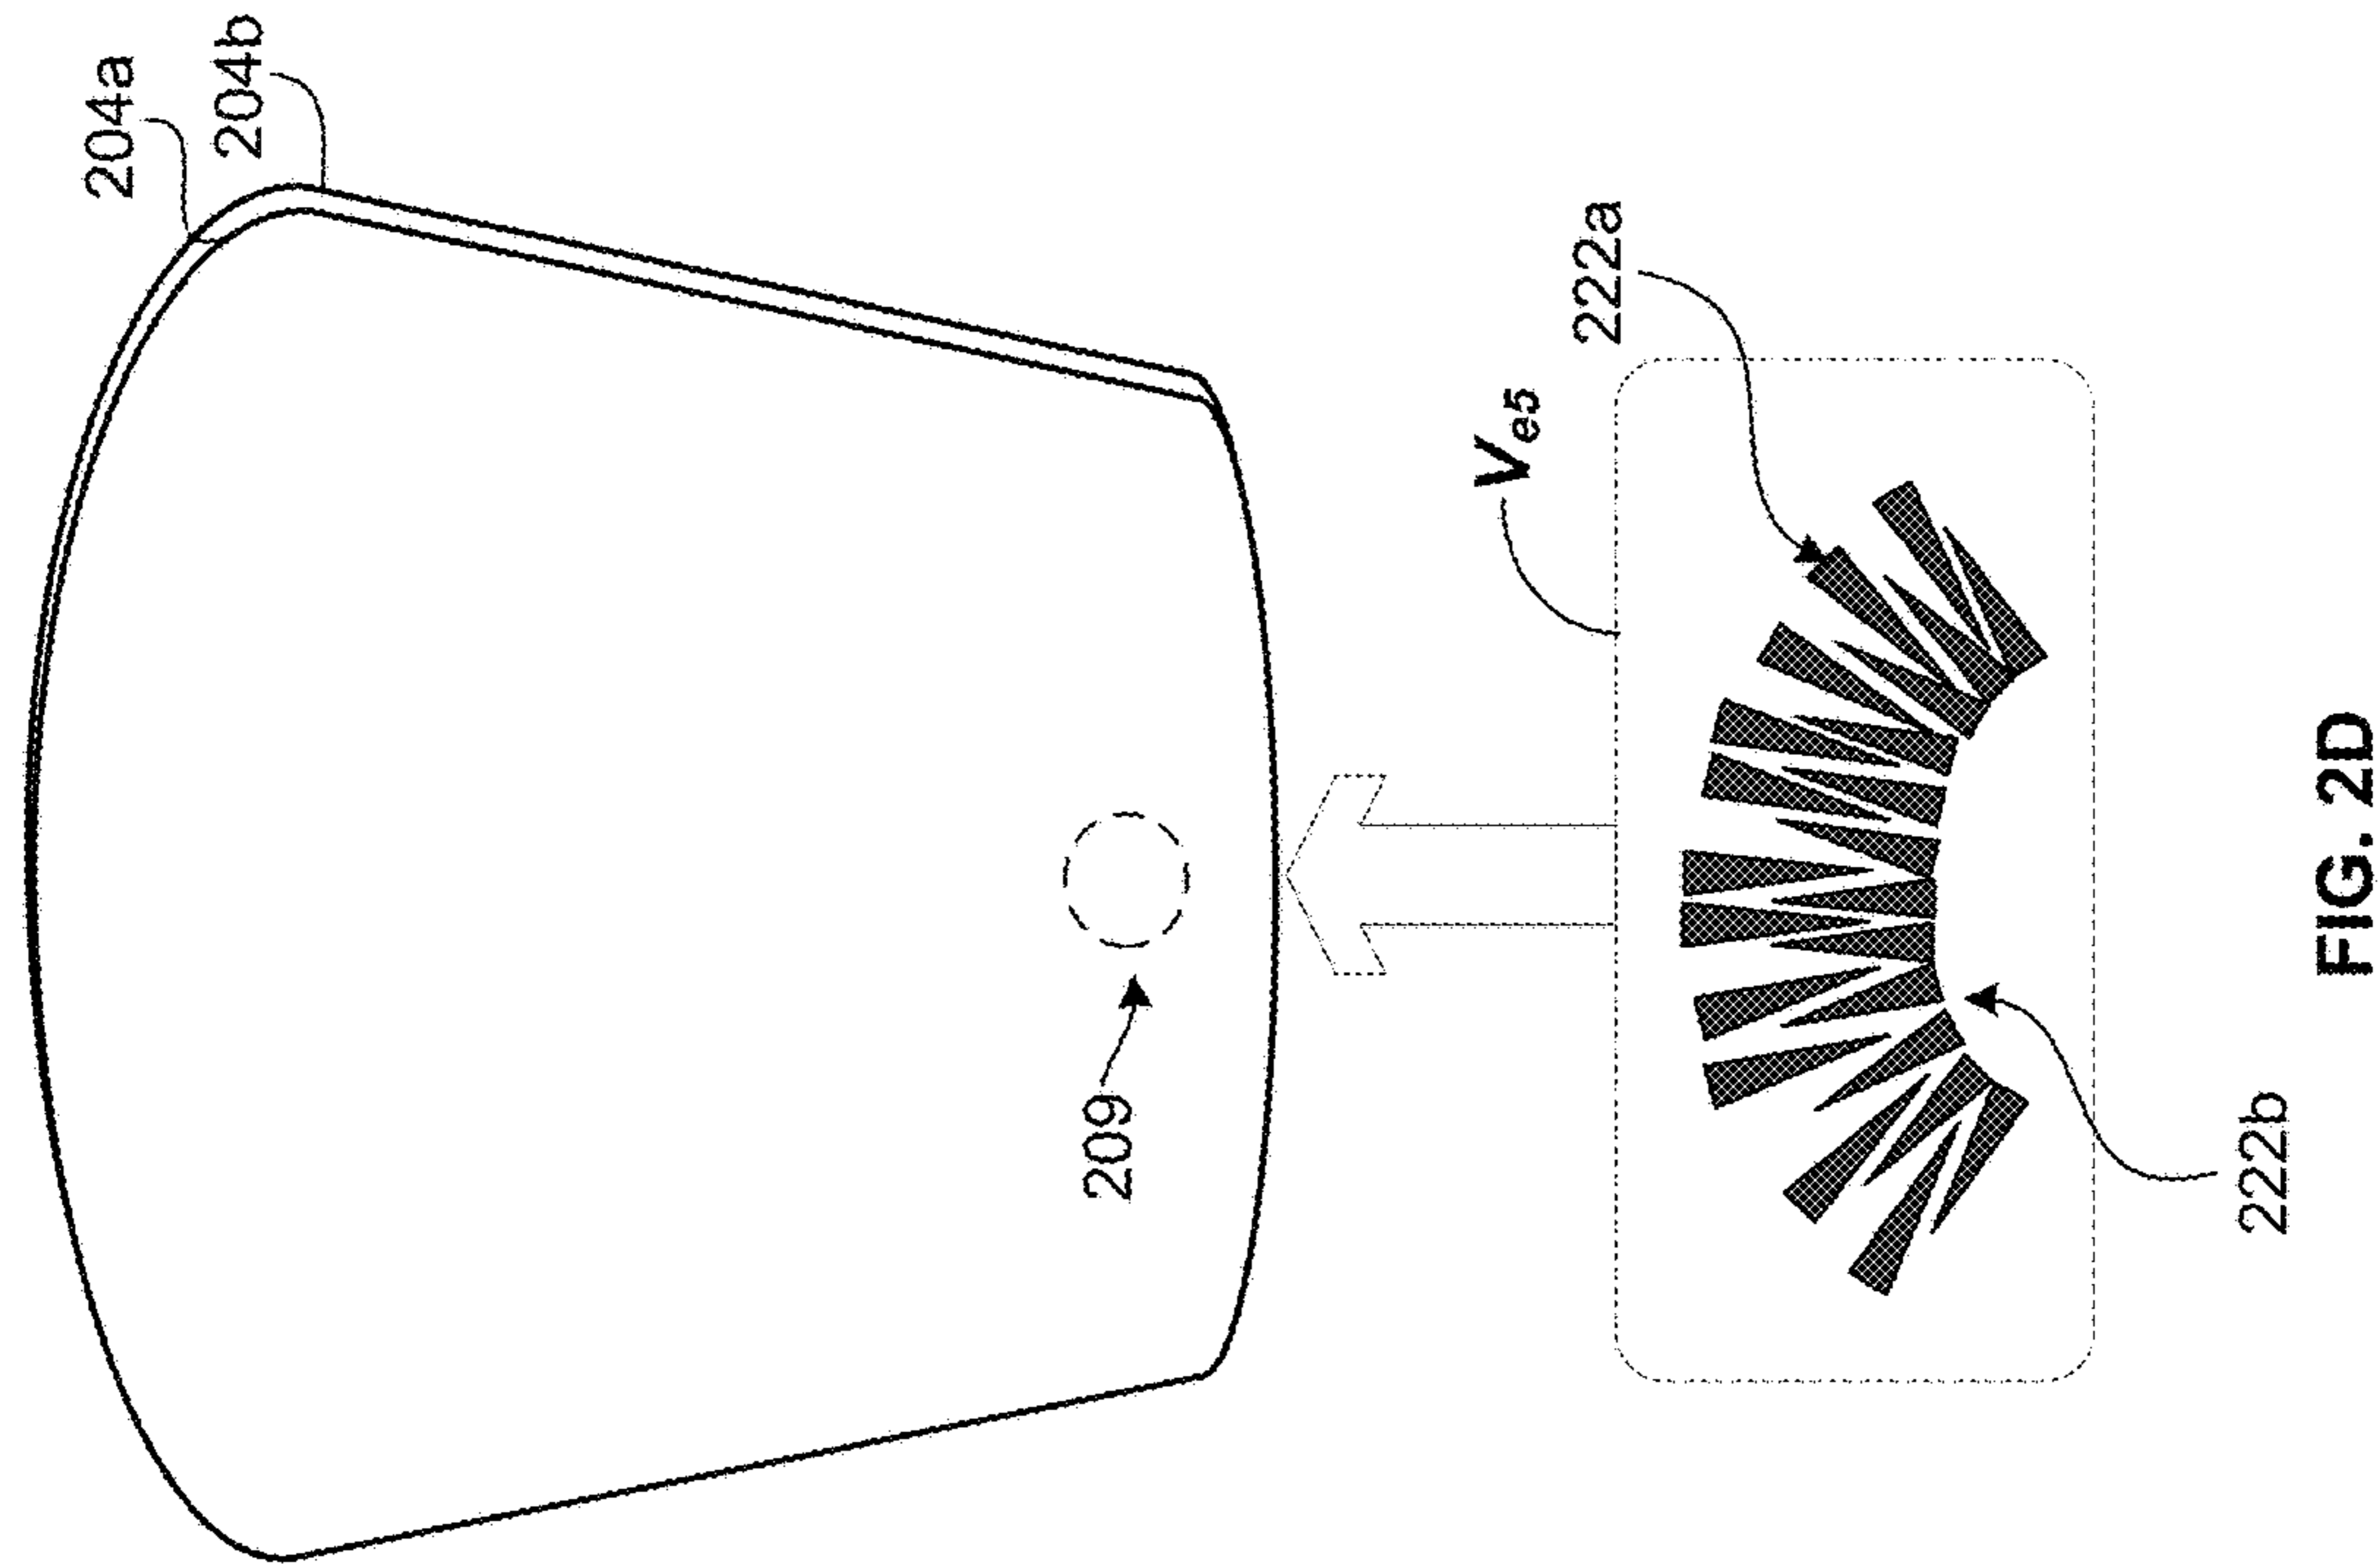


FIG. 2D

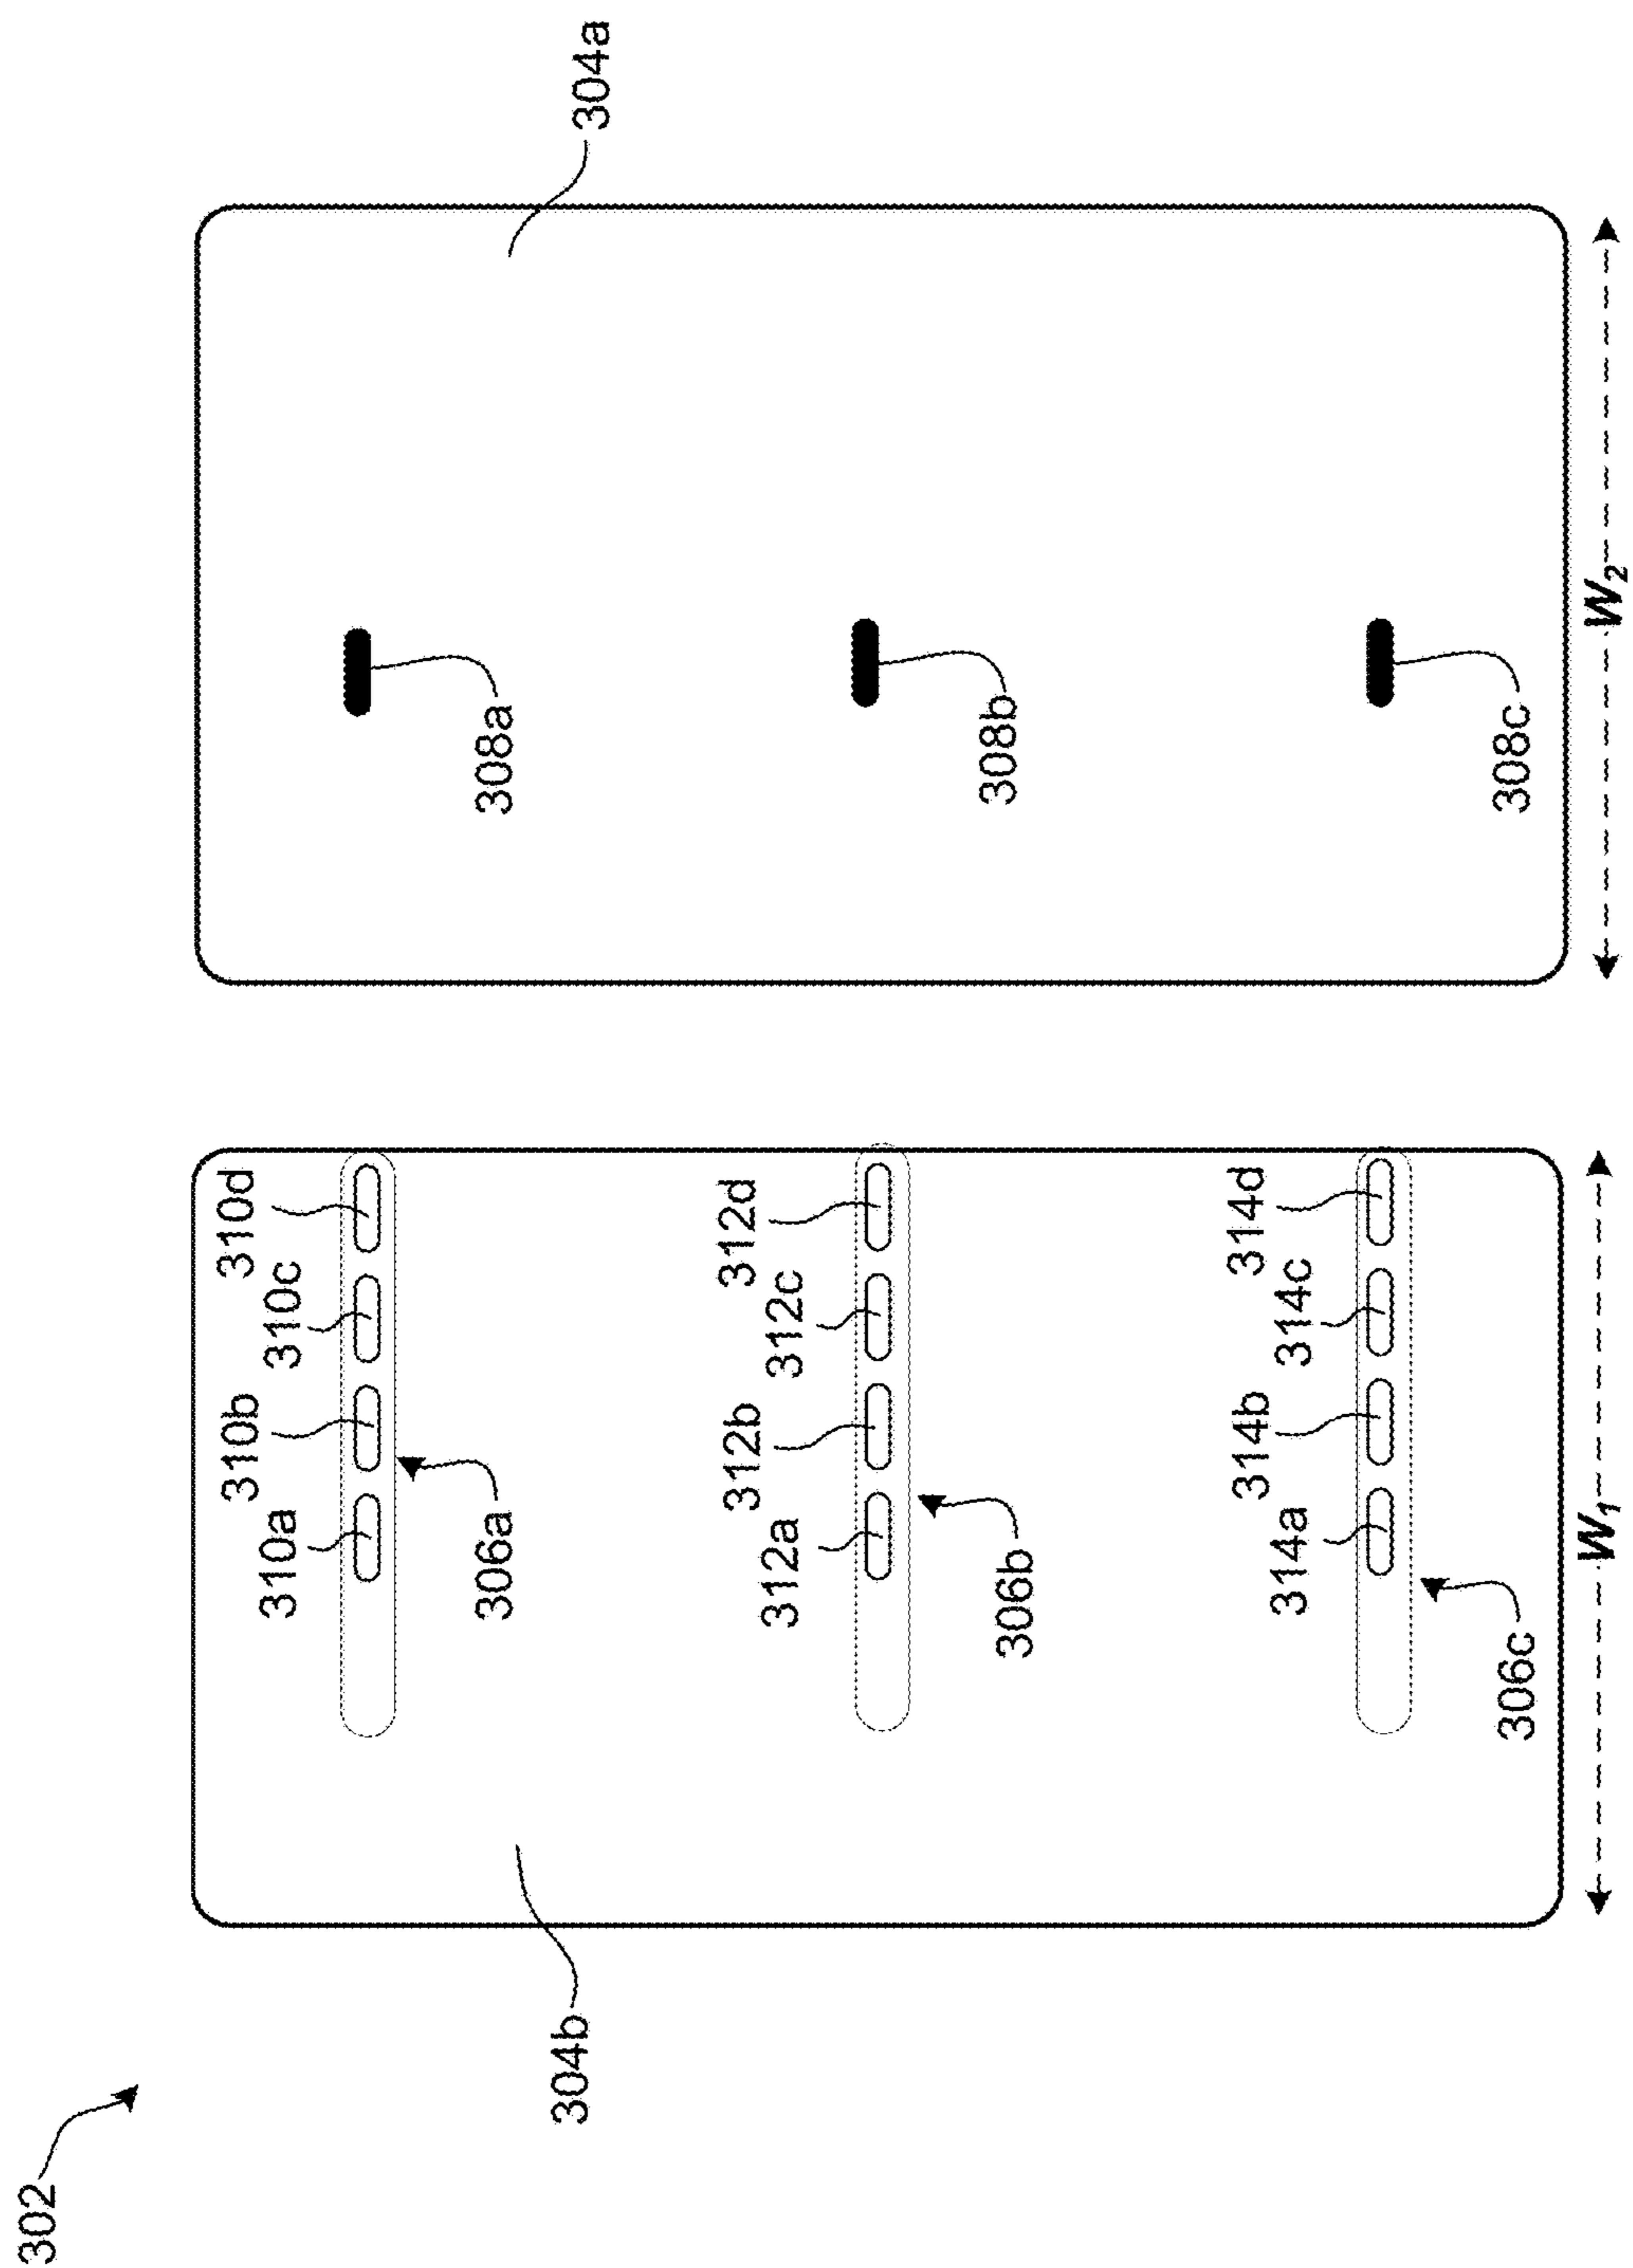


FIG. 3A

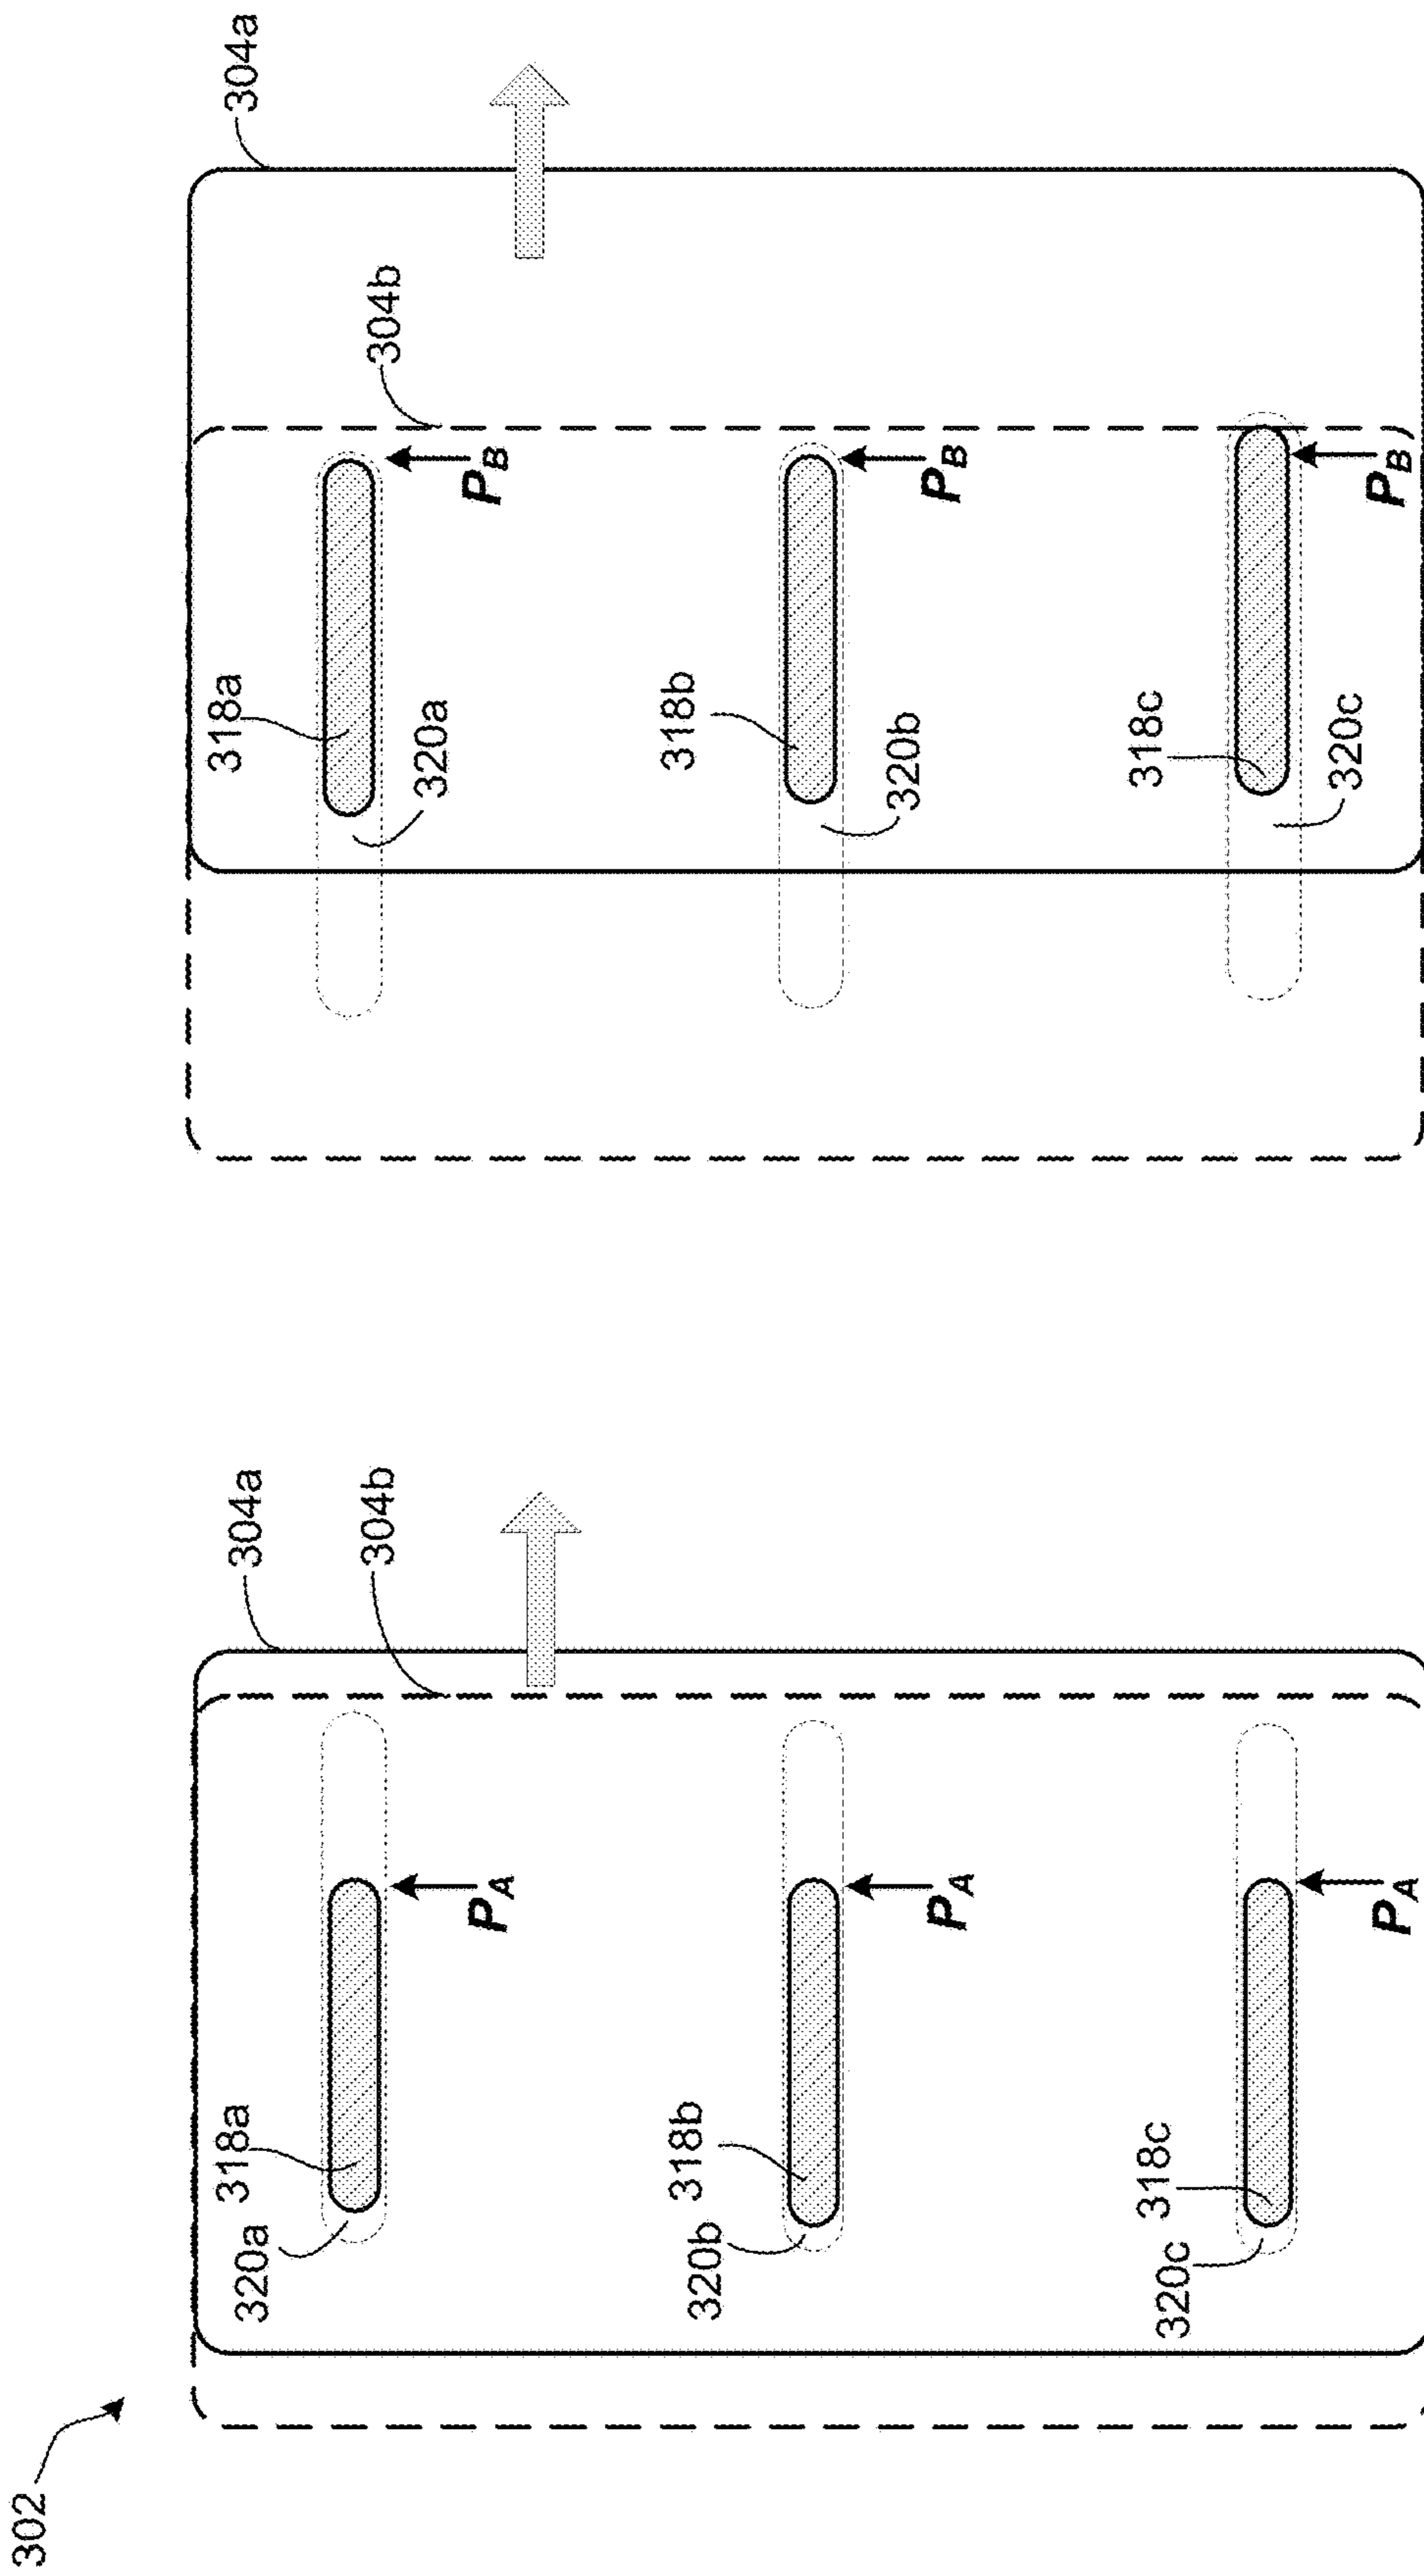


FIG. 3C

FIG. 3B

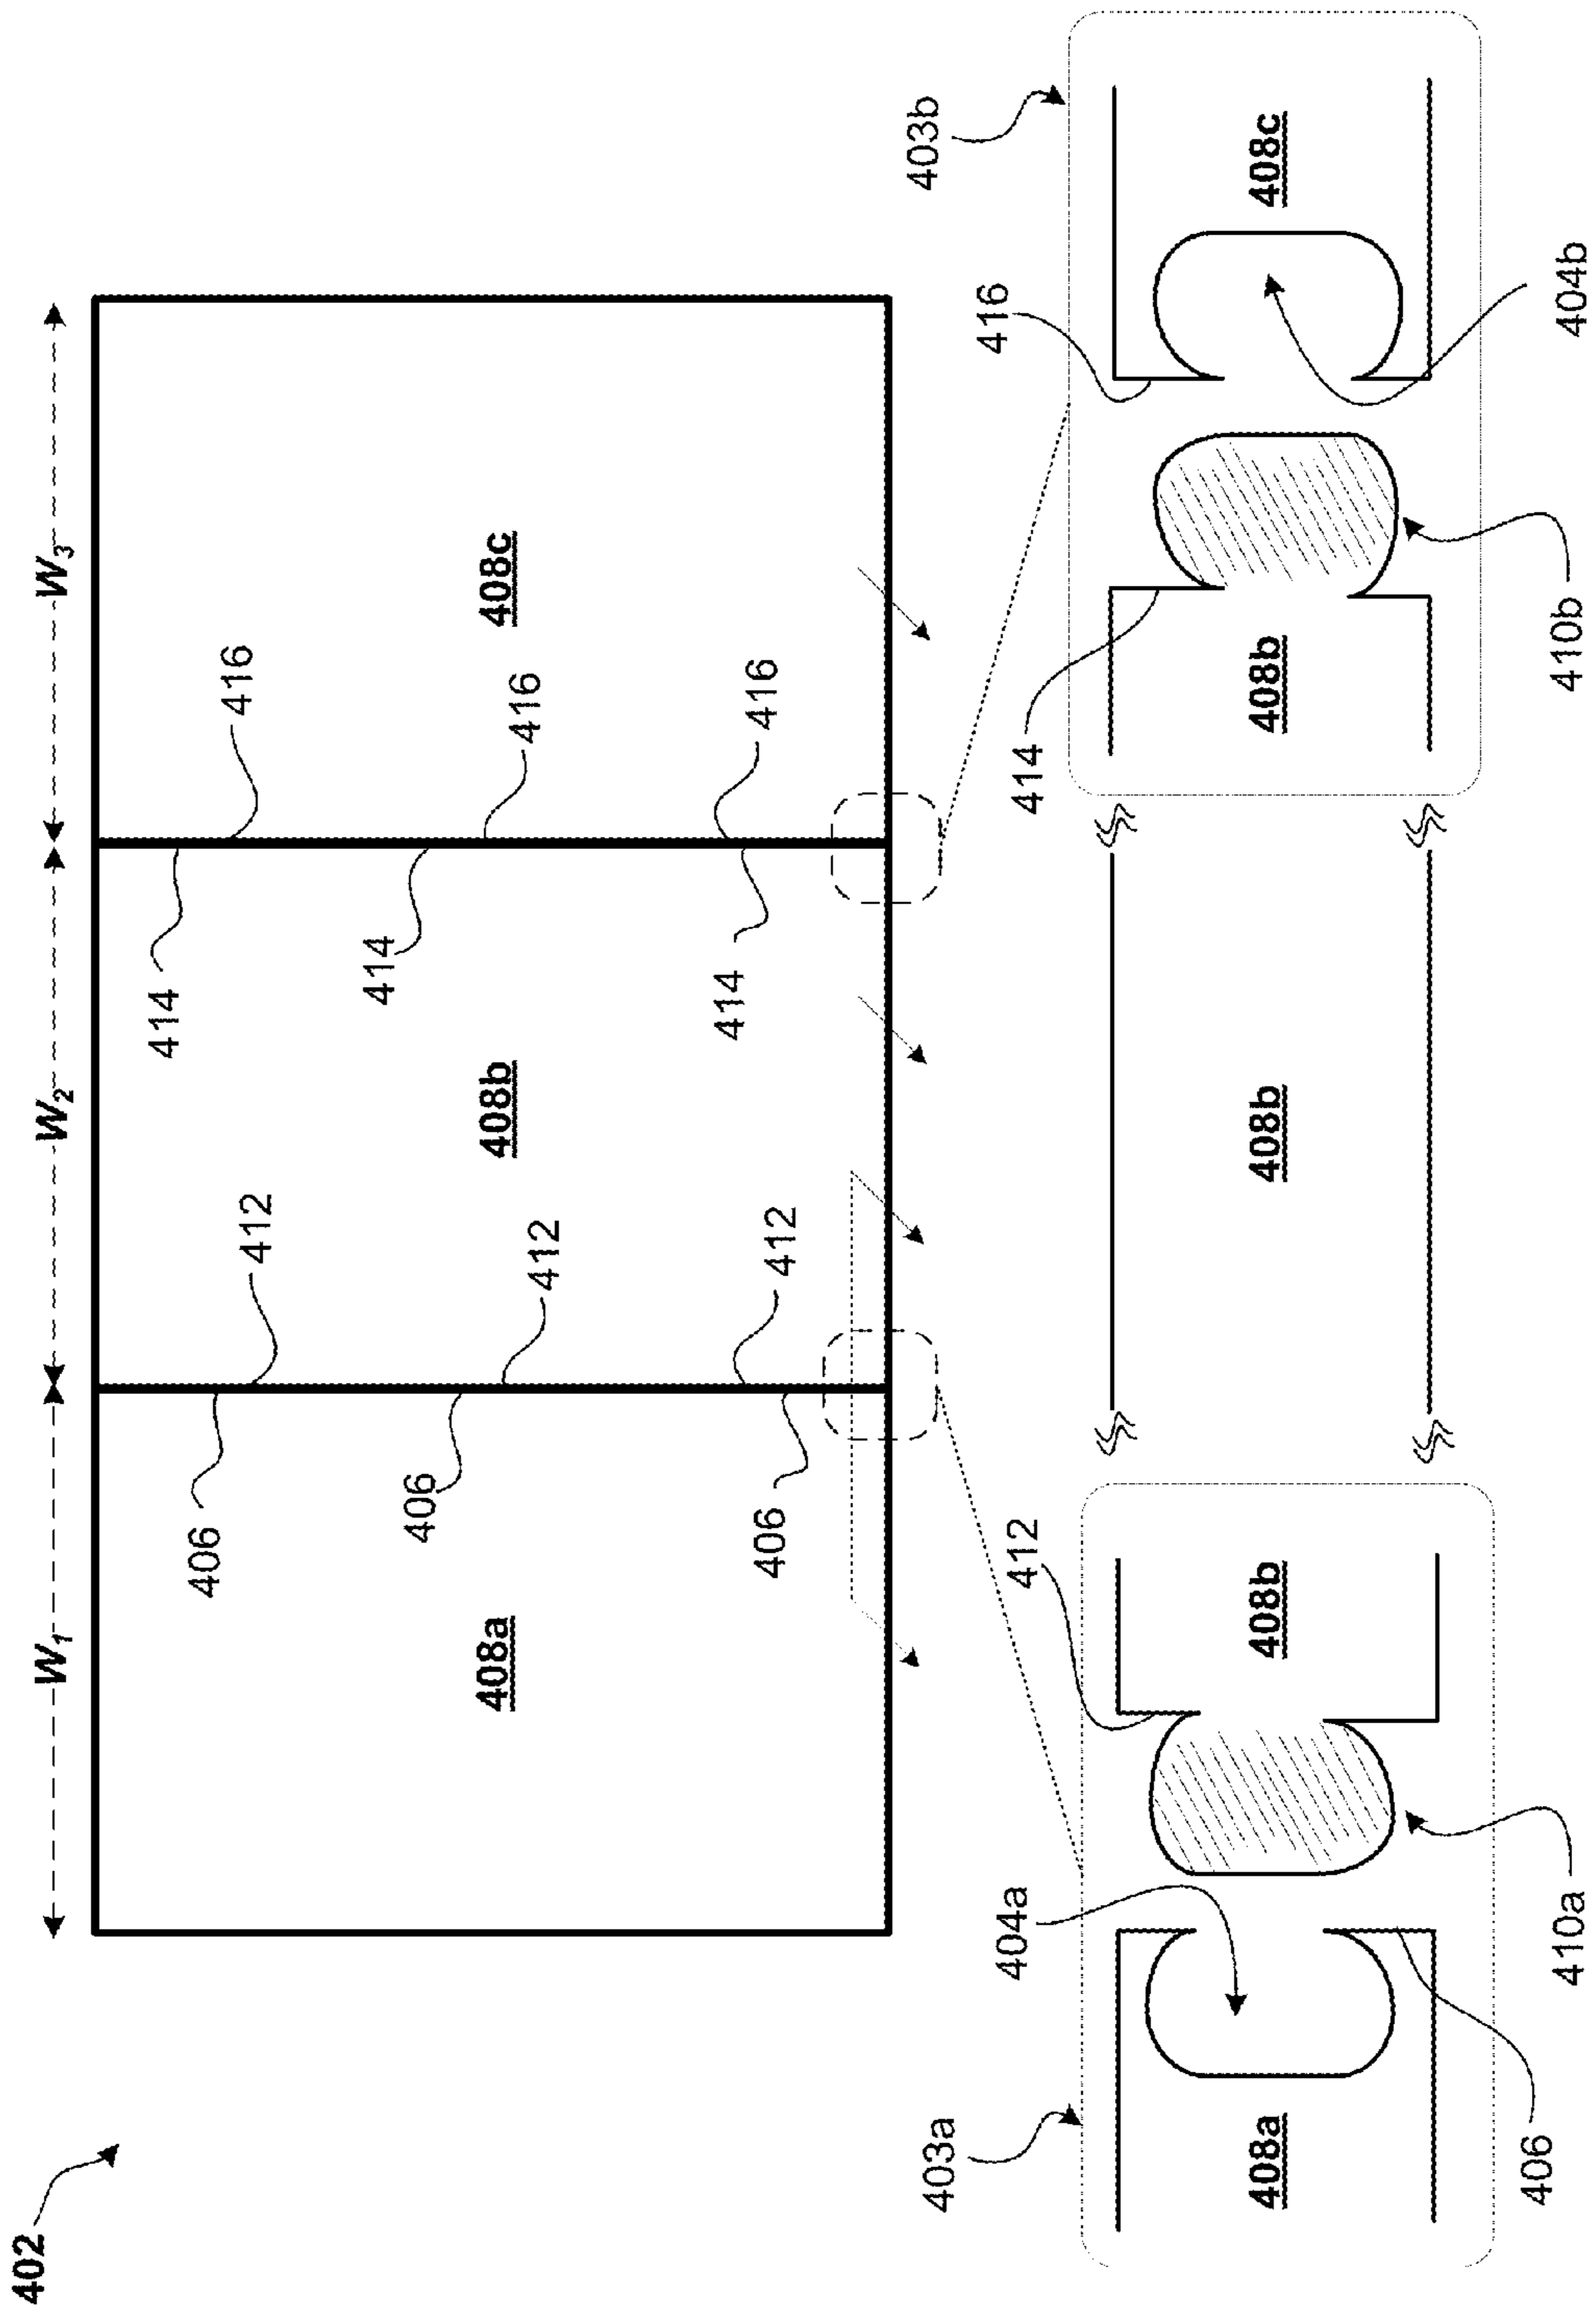


FIG. 4A

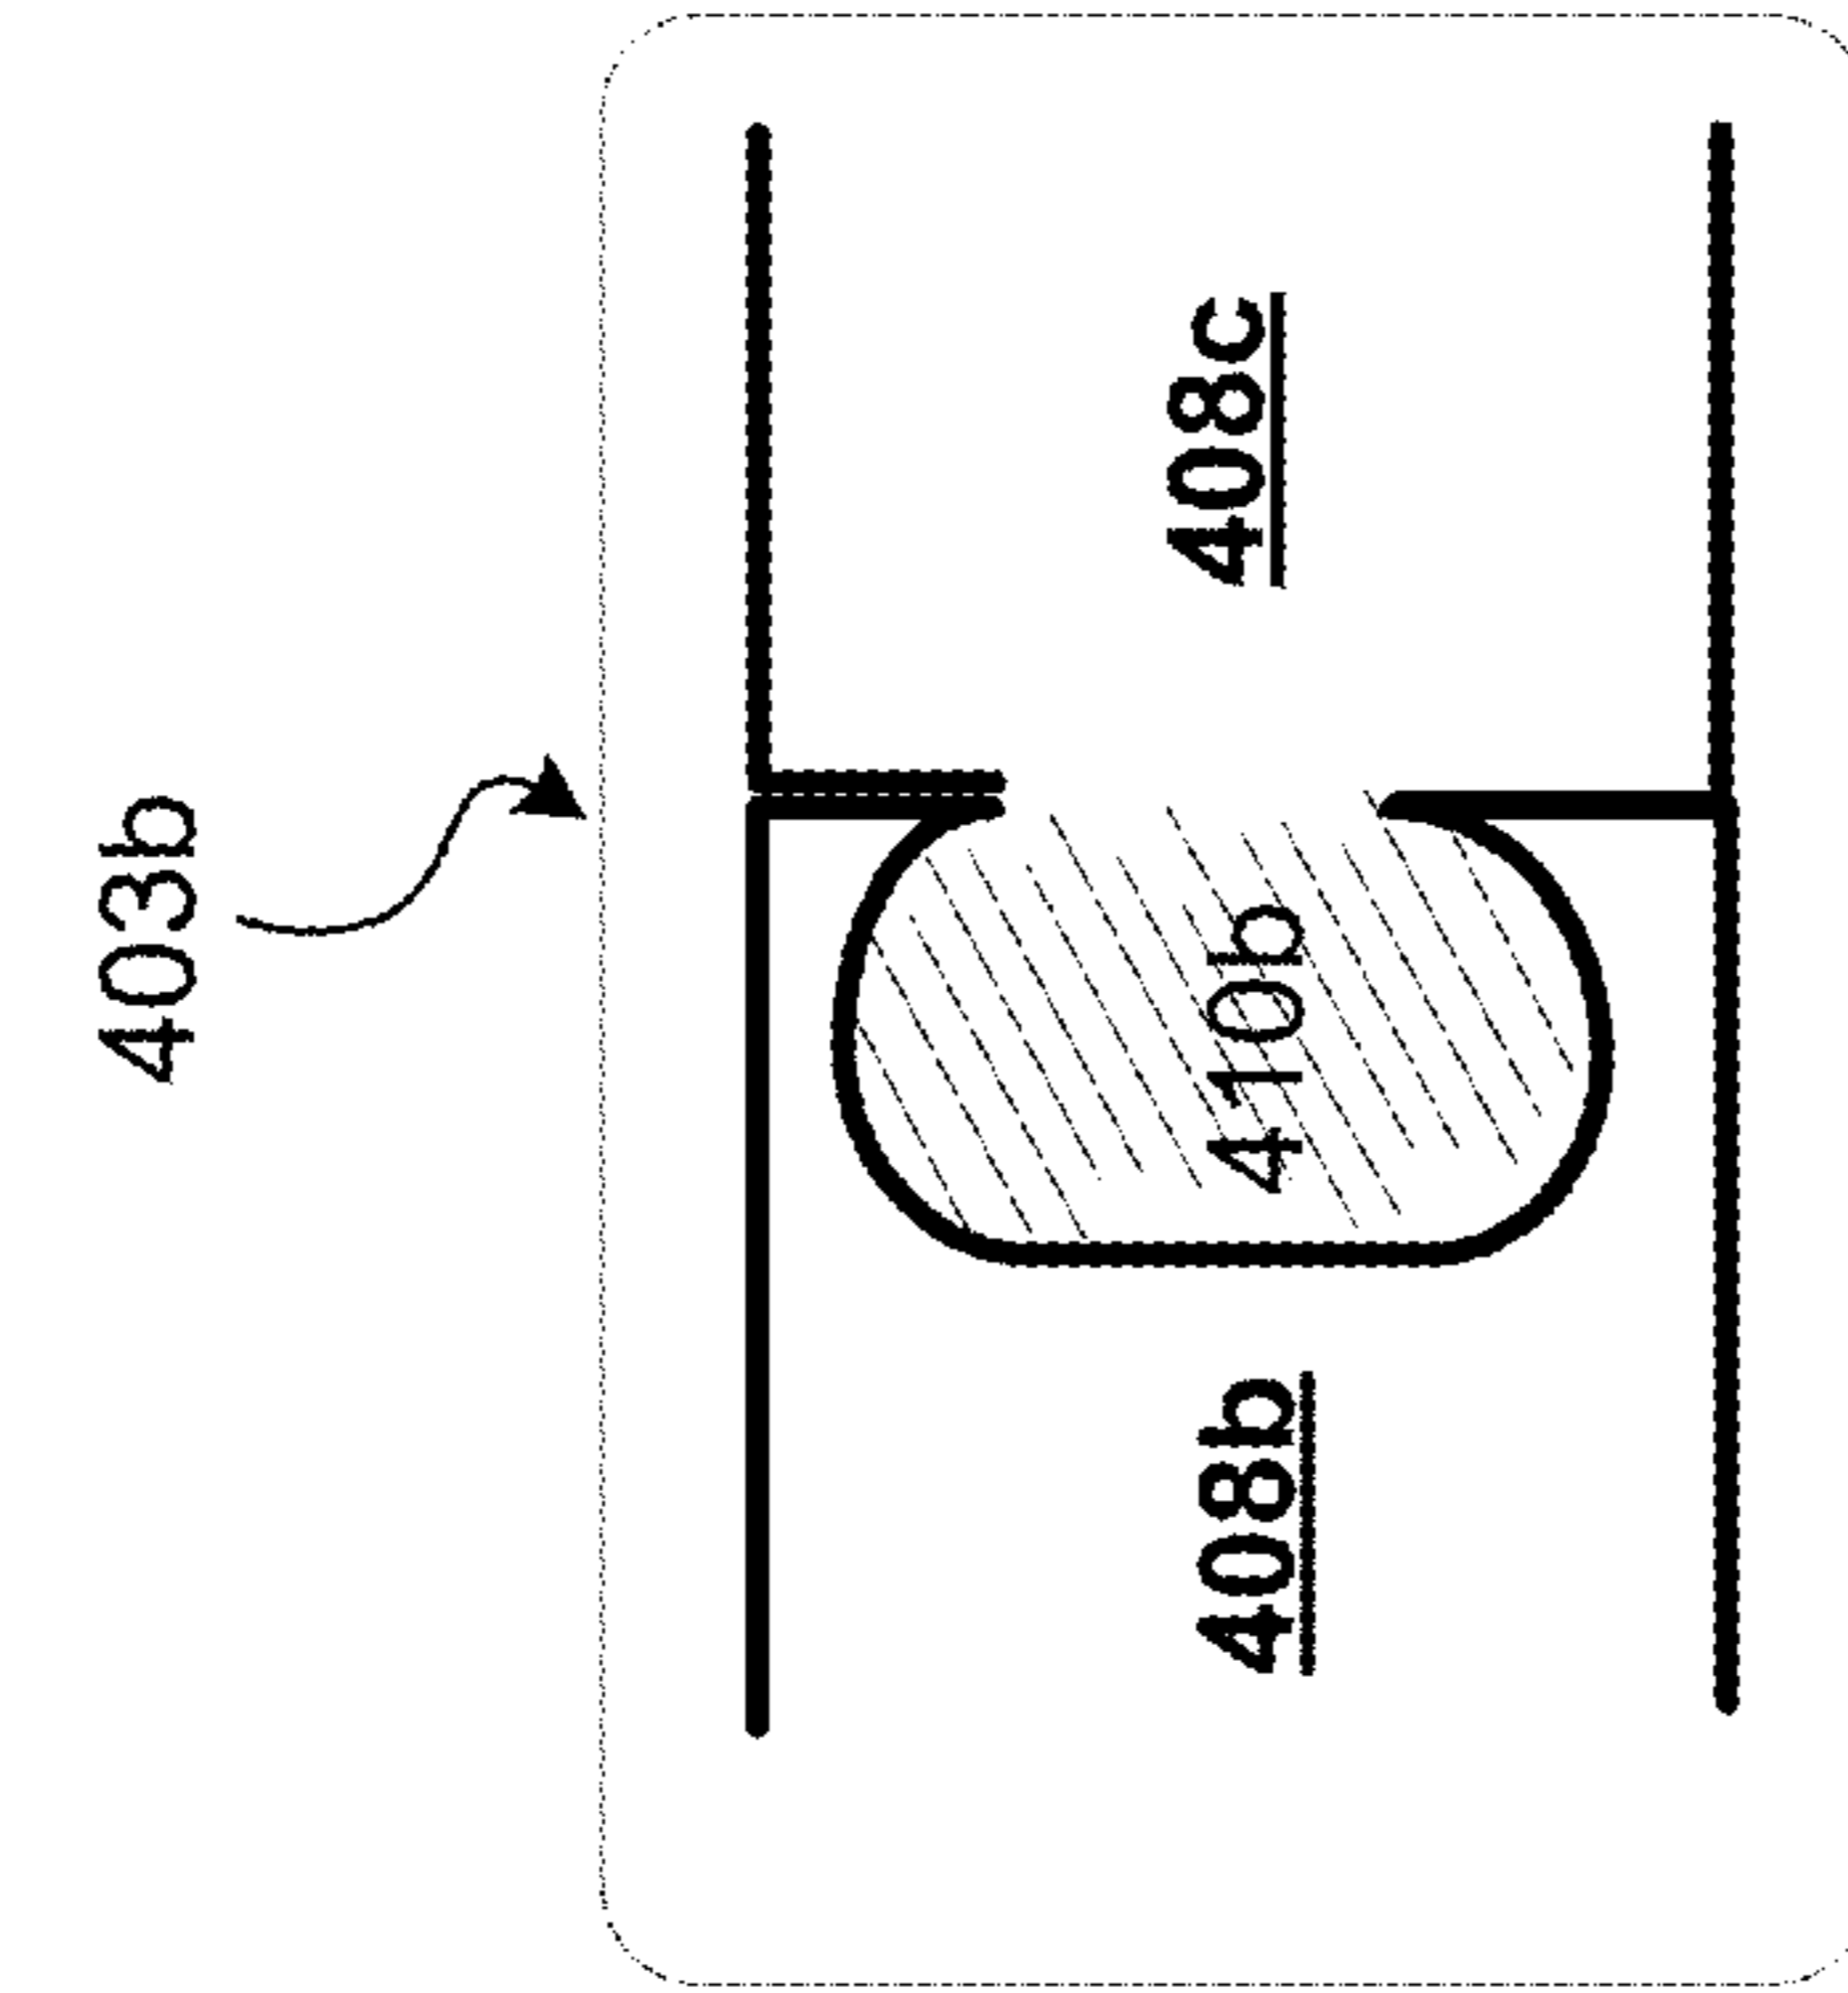


FIG. 4B

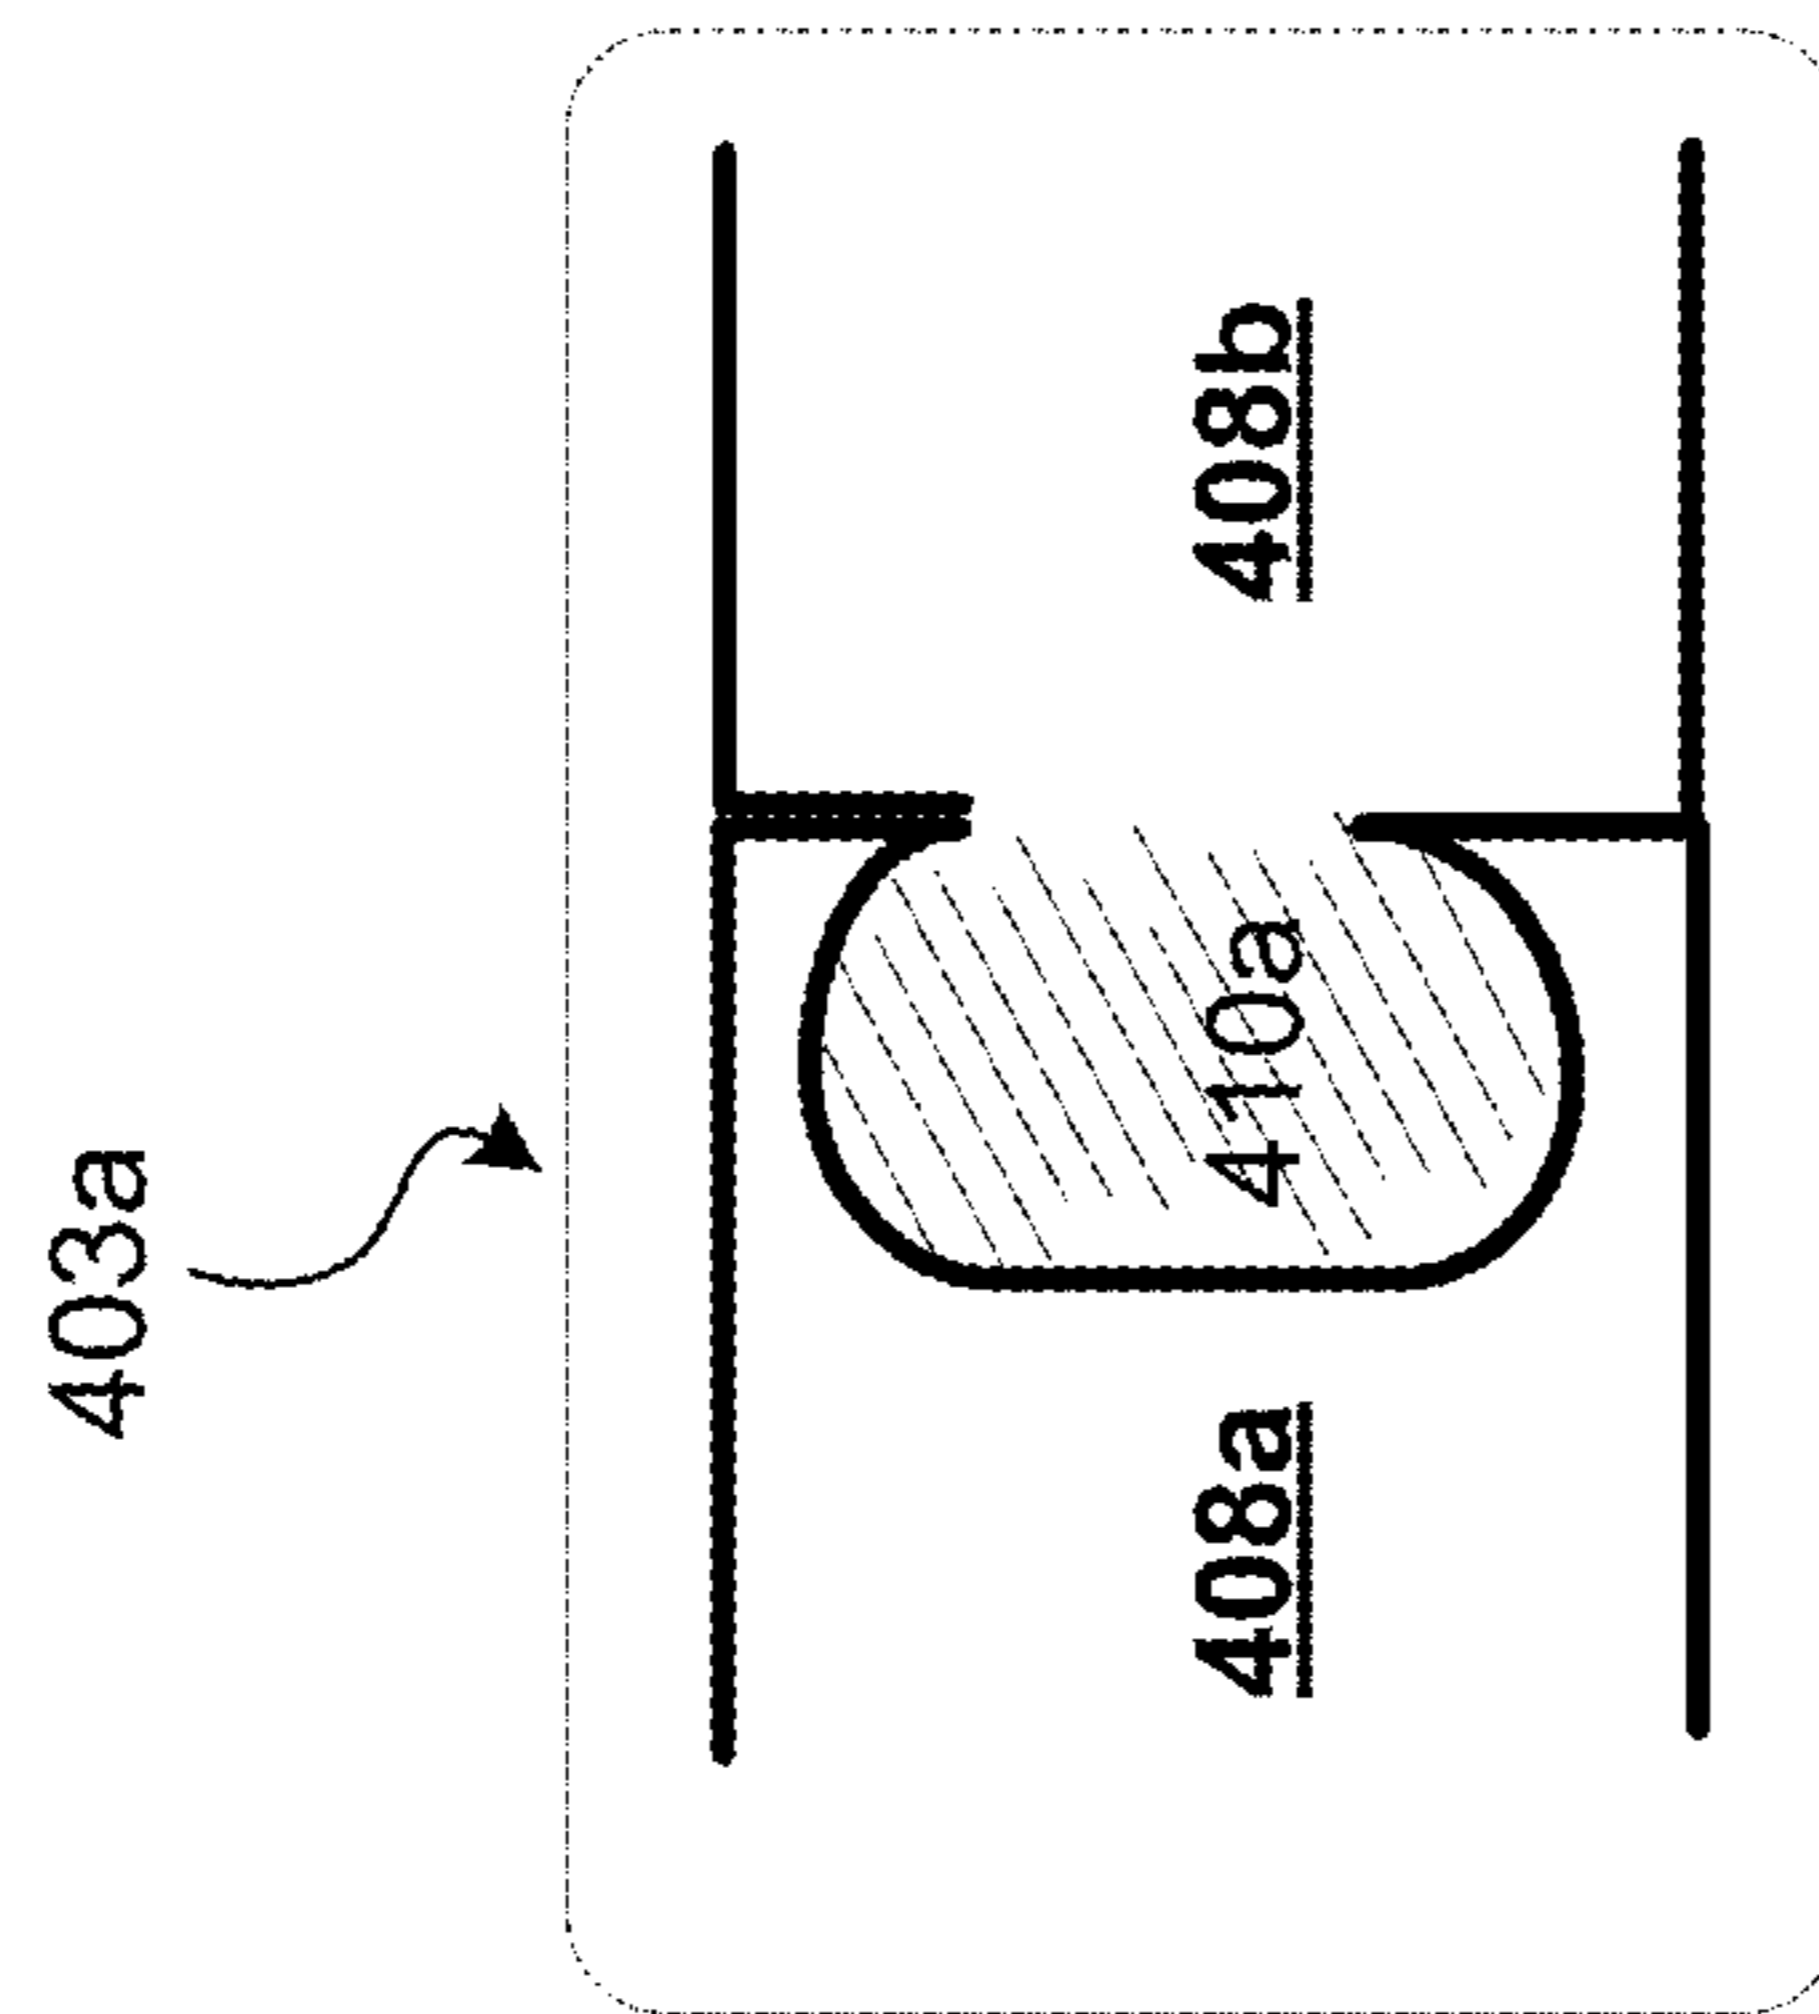


FIG. 4C

1

EXPANDABLE SURGICAL IMPLANT DEVICE

CROSS-REFERENCE TO RELATED APPLICATION

This application is a continuation of and claims priority under 35 USC. § 120 from application Ser. No. 13/959,538, filed on Aug. 5, 2013, herein incorporated by reference in its entirety.

BACKGROUND

a. Field of the Invention

The present invention generally relates to medical devices, and particularly to surgical implants.

b. Background of Invention

A vast number of surgical procedures require the application of one or more surgical incisions on the patient's body in order allow the medical specialist (e.g., surgeon) to access an area-of-interest. Moreover, in many instances, implant devices may be used to repair or replace an existing component of the body.

For example, in the field of ophthalmology, fracture and damage to the floor or wall(s) of the eye socket (i.e., orbit) as a result of trauma may necessitate the placement of an implant device over the fractured and damaged area.

However, it may be appreciated that generally, the length of the incision used to insert an implant may be proportional to the greatest physical dimension of the implant device needed to address the medical issue. For example, if an applied incision is too small, a requisite implant may not fit through such an incision.

It may, therefore, be advantageous to, among other things, provide implant devices that facilitate smaller incisions and consequently less surgical trauma, less chance for complications, and faster recovery.

BRIEF SUMMARY

According to at least one exemplary embodiment, a surgical implant device may include a first substantially planar portion having a first surface area, a second substantially planar portion having a second surface area, and a coupling device for connecting the first substantially planar portion to the second substantially planar portion. The coupling device facilitates expanding and contracting the first and the second substantially planar portion to provide an implant surface area corresponding to the first surface area during insertion of the surgical implant within an incision, and having a third surface area corresponding to both the first surface area and at least a portion of the second surface area following insertion of the surgical implant within the incision.

According to another exemplary embodiment, a method of implanting a surgical implant device having an expandable surface area may include making an incision of a first width for implanting the surgical implant device and adjusting the expandable surface area of the surgical implant device to a reduced surface area such that the reduced surface area causes the surgical implant to have a second width that is less than, or substantially the same as, the first width. The surgical implant device having the reduced surface area is placed into the incision. The expandable surface area of the surgical implant device is then adjusted to an increased surface area following the placement of the

2

surgical implant device, such that the reduced surface area causes the surgical implant to have a third width greater than the second width.

According to yet another exemplary embodiment, a method of implanting a surgical implant device may include making an incision of a first width for implanting the surgical implant device. A first substantially planar component associated with the surgical implant device may then be placed into the incision, whereby the first substantially planar component includes a second width that is less than or substantially the same as the first width. Similarly, a second substantially planar component associated with the surgical implant device may be placed into the incision, whereby the second substantially planar component includes a third width that is less than or substantially the same as the first width. The first substantially planar component is coupled to the second substantially planar component, whereby the first substantially planar component includes a first surface area and the second substantially planar component includes a second surface area. The coupling accordingly provides a surface area corresponding to the sum of the first and the second surface areas.

BRIEF DESCRIPTION OF THE SEVERAL VIEWS OF THE DRAWINGS

FIG. 1A illustrates a surgical implant device according to an exemplary embodiment;

FIG. 1B illustrates the insertion of the surgical implant device of FIG. 1A according to an exemplary embodiment;

FIG. 2A depicts an expandable surgical implant device in an unexpanded state according to one exemplary embodiment;

FIG. 2B depicts the expandable surgical implant device of FIG. 2A in an expanded state;

FIG. 2C depicts an exemplary embodiment of a coupling device for providing rotatable coupling and positional retention between top and bottom planar surfaces of the expandable surgical implant device of FIG. 2A;

FIG. 2D depicts the interlocking of the top and bottom planar surface of the surgical implant device of FIG. 2A in an unexpanded state using interlocking fins according to one exemplary embodiment;

FIG. 2E depicts the interlocking of the top and bottom planar surface of the surgical implant device of FIG. 2A in an expanded state using the interlocking fins according to one exemplary embodiment;

FIG. 3A depicts an expandable surgical implant device according to another exemplary embodiment;

FIG. 3B depicts a modified exemplary embodiment of the expandable surgical implant device of FIG. 3A in a substantially unexpanded state;

FIG. 3C depicts the modified exemplary embodiment of the expandable surgical implant device of FIG. 3A in a substantially expanded state;

FIG. 4A depicts an expandable surgical implant device according to yet another exemplary embodiment;

FIG. 4B depicts a first mating receptacle and mating connector for the expandable surgical implant device of FIG. 4A; and

FIG. 4C depicts a second mating receptacle and mating connector for the expandable surgical implant device of FIG. 4A.

The drawings are not necessarily to scale. The drawings are merely schematic representations, not intended to portray specific parameters of the invention. The drawings are

intended to depict only typical embodiments of the invention. In the drawings, like numbering represents like elements.

DETAILED DESCRIPTION

According to the following described embodiments, expandable implant devices may be used in order to reduce surgical incision size (e.g., width) for the placement of implants within the body.

Referring to FIG. 1A, a surgical implant device **102** according to an exemplary embodiment is depicted. The surgical implant device **102** is inserted into an incision **104** created by a medical professional (e.g., surgeon), whereby the width, as defined by A, of the surgical implant device **102** may be substantially the same as the width, as defined by B, of the created incision **104**. In some implementations, for example, the width A of the surgical implant device **102** may be less than the width B of the created incision **104**.

Referring to FIG. 1B, the inserted surgical implant device **102** may be utilized to cover or support an injury, as depicted by **106**. According to one non-limiting example, the injury **106** may include a fracture in the floor **108** of an orbital implant. As illustrated, the geometric size of the surgical implant device **102** is selected to be in proportion to the area or size of the injury **106**. Thus, the surgical implant device **102** may completely cover the injury **106** (i.e., fracture) in the orbital floor **108**. Consequently, the incision width B is created to accordingly facilitate the insertion of the surgical implant device **102**. Thus, the larger the surgical implant device **102** is, the larger the corresponding incision **104** needs to be. However, as depicted and described in the following paragraphs, a surgical implant device may be expanded to cover a larger injury.

Referring to FIG. 2A, one embodiment of an expandable surgical implant device **202** is depicted. In an unexpanded state, surgical implant device **202** may include a width, as defined by C. Thus, surgical implant device **202** may be inserted into, for example, incision **104** (FIG. 1A) based on the width C of the surgical implant device **202** being substantially the same as or smaller than the width B of the incision **104** (FIG. 1A). Referring to FIG. 2B, however, in an expanded state, surgical implant device **202** may be manipulated to a larger width area, as defined by D, once the surgical implant device **202** is placed within the incision **104** (FIG. 1B).

For example, if an injury **107** (FIG. 1B) is more extensive and, thus, extends over a greater area of the orbital floor or wall **108** (FIG. 1B) compared to injury **106** (FIG. 1B), the surgical implant device **202** may be expanded to width D in order to have a larger surface area compared to when the surgical implant device **202** has a smaller surface area in the unexpanded state (i.e., at width C). The larger surface area of the surgical implant device **202** may now facilitate covering the more extensive injury **107** (FIG. 1B) without the disadvantage associated with the requisite need for creating a larger incision relative to incision **104** (FIG. 1B). Thus, a smaller incision width (e.g., FIG. 1B: width B) may be created for larger injuries (e.g., FIG. 1B: incision **107**) by inserting a surgical implant device in an unexpanded state (e.g., FIG. 2A: device **202**) having a smaller width (e.g., FIG. 2A: width C), and subsequently expanding the surface area and width (e.g., FIG. 2B: width D) of the surgical implant device (e.g., FIG. 2B: device **202**) to cover the larger injury once the device has been inserted.

As depicted in FIG. 2A, in the unexpanded state, the surgical implant device **202** may include two substantially

planar surfaces that almost entirely overlap. As shown, the top planar surface **204a** and the bottom planar surface **204b** are completely overlapping such that only top planar surface **204a** is visible in FIG. 2A. Referring to FIG. 2B, the top planar surface **204a** and the bottom planar surface **204b** may be rotatably manipulated, as indicated by arrow A_r , such that the top planar surface **204a** and the bottom planar surface **204b** fan-out to partially overlap. Therefore, as illustrated, the total surface area of the manipulated surgical implant device **202** increases to the sum of the surface area of the top planar surface **204a** and at least a portion A_p of the surface area of the bottom planar surface **204b**.

Referring to FIG. 2A, region **206** of the surgical implant device **202** may, for example, include a coupling device (e.g., see FIG. 2C) that both provides a rotatable coupling and positional retention capability between the top planar surface **204a** and the bottom planar surface **204b**. Referring to FIG. 2B, a swiveling mechanism **208** may rotatably couple the top planar surface **204a** and the bottom planar surface **204b** of the surgical implant device **202**. The following paragraphs provide non-limiting examples of various coupling devices that facilitate the expansion and contraction of implant devices for the purposes of mitigating the need for increased incision sizes that correspond to the area/size of the injury.

Referring to FIG. 2C, an embodiment of a coupling device **210** for providing rotatable coupling and positional retention between top planar surface **204a** and bottom planar surface **204b** is depicted. The coupling device **210** may include a swiveling mechanism **209** having a snap fit receptacle **212** located on the bottom planar surface **204b** and a snap fit connector **214** located on the top planar surface **204a**. As illustrated, the expanded view V_{e1} of snap fit receptacle **212** shows a cylindrical opening **216** that is adapted to receive a connector, whereby the connector has the ability to swivel or rotate within the opening **216**. The expanded view V_{e2} of snap fit connector **214** shows a cylindrical plug **218** that is adapted to receive a connector, whereby the connector has the ability to swivel or rotate within the opening **216**.

The snap fit receptacle **212** also includes coupling region **220b** while snap fit connector **214** also includes coupling region **220a**. In operation, the snap fit connector **214** is pushed into snap fit receptacle **212** in the direction of arrow A_f . Thus, the coupling region **220a** of snap fit receptacle **212** may be forcibly pushed into the cylindrical opening **216** of snap fit receptacle **212** such that coupling region **220a** elastically deforms to accommodate the smaller cross-section of the cylindrical opening **216**. As coupling region **220a** fills coupling region **220b** of the snap fit receptacle **212**, coupling region **220a** elastically expands back to its original non-deformed state. Since the coupling regions **220a**, **220b** are now mated and have a larger cross-section than the cylindrical opening **216**, the snap fit receptacle **212** and the snap fit connector **214** remain coupled together. Thus, the top planar surface **204a** and the bottom planar surface **204b** are coupled together and may accordingly rotate about the mated snap fit receptacle **212** and connector **214**.

The volume and shape of the snap fit connector **214** is substantially the same as, or slightly less than, that of the snap fit receptacle **212** and, therefore, the snap fit connector **214** has the ability to rotate or swivel within the snap fit receptacle **212**. The snap fit connector **214** may include a flexible polyethylene material that enables it to deform when forcibly inserted into the snap fit receptacle **212**. Moreover, the top planar surface **204a** and the bottom planar surface

204b may include a thickness of about 0.6-1.5 millimeters and each may have an embedded titanium mesh.

In order to maintain the top planar surface **204a** and the bottom planar surface **204b** in a set position after rotation, an interlocking mechanism including a plurality of interlocking fins **222a**, **222b** corresponding to the top and the bottom planar surfaces **204a**, **204b** may be utilized. As depicted in expanded view V_{e3} , the interlocking fins **222a** of the top planar surface **204a** may have a substantially downward orientation. Particularly, the substantially downward orientation of the interlocking fins **222a** is relative to the plane of surface **204a**. Also, as shown in expanded view V_{e4} , the interlocking fins **222b** of the bottom planar surface **204b** may include a substantially upward orientation. Particularly, the substantially upward orientation of the interlocking fins **222b** is accordingly relative to the plane of surface **204b**.

Referring to FIG. 2D, while the top planar surface **204a** and the bottom planar surface **204b** of the surgical implant device **202** are in a substantially unexpanded state, as depicted in expanded view V_{e5} , the fins of interlocking fins **222a** and **222b** overlap almost entirely and interlock. Referring to FIG. 2C, as the top and bottom planar surfaces **204a**, **204b** of the surgical implant device **202** are forcibly manipulated (i.e., along arrow A_r) into an expanded state using the swiveling mechanism **209**, as depicted in expanded view V_{e6} , the top planar surface **204a** interlocking fins **222a** are repositioned relative to the bottom planar surface **204b** interlocking fins **222b**.

Although the fins are flexible enough to allow for such repositioning, absent a sufficient external force, the engaged interlocking fins **222a**, **222b** remain partially overlapping and maintain the expanded position of the top and bottom planar surfaces **204a**, **204b** of the surgical implant device **202**. This may be required since, for example, once the surgical implant device **202** is placed within a patient's incision, the bodily movements of the patient can cause the surgical implant device **202** to contract or collapse from its expanded state. Thus, the interlocking mechanism including the plurality of interlocking fins **222a**, **222b** avoids such a collapse or contraction of the surgical implant device **202**. However, following a finite duration after placement of the surgical implant device **202**, the top and bottom expanded planar surfaces **204a**, **204b** become less susceptible to inadvertent repositioning due to external forces. This may be due to the bio-integration of the surgical implant device **202** within the patient's body and the healing processes corresponding to the surrounding tissue associated with the surgical implant device **202**.

In addition, for an orbital implant example, the top and the bottom expanded planar surfaces **204a**, **204b** may include relative coarse outer surfaces, whereby the coarseness of the outer surfaces enhance the contact stability of the surgical implant device **202** with the orbital floor under the periosteum. Also, in the orbital implant example, the top and bottom expanded planar surface **204a**, **204b** may include relative smooth outer surfaces, whereby the smoothness of the outer surfaces in contact with the periosteum avoids and/or mitigates any movement inhibitions with the respect to the eyeball located over the surgical implant device **202**.

Referring to FIG. 3A, another exemplary embodiment of an expandable surgical implant device **302** is depicted. The expandable surgical implant device **302** may include a top planar surface **304a** and a bottom planar surface **304b**. The bottom planar surface **304b** may include a plurality of snap fit receptacles **306a-306c**, while the top planar surface **304a** may accordingly include a plurality of corresponding snap fit connectors **308a-308c** for engaging any one of the

openings within snap fit receptacles **306a-306c**. As illustrated, each of the plurality of snap fit receptacles **306a-306c** may include several openings. For example, snap fit receptacle **306a** includes openings **310a-310d** and snap fit receptacle **306b** includes openings **312a-312d**. Similarly, snap fit receptacle **306c** includes openings **314a-314d**. In operation, the snap fit connector **308a** of top planar surface **304a** may couple to any one of the openings **310a-310d** within snap fit receptacle **306a**. Snap fit connector **308b** of top planar surface **304a** may couple to any one of the openings **312a-312d** within snap fit receptacle **306b**. Also, snap fit connector **308c** of top planar surface **304a** may couple to any one of the openings **314a-314d** within snap fit receptacle **306c**.

By providing the ability to couple the top planar surface **304a** and the bottom planar surface **304b** in the described manner, each planar surface may be individually inserted into an incision of substantially the same width as either planar surface, and subsequently coupled together within the region of the body receiving the expandable surgical implant device **302**. For example, the bottom planar surface **304b** having a width of W_1 may be inserted into incision **104** (FIG. 1B) having a width B , whereby the width of W_1 of the bottom planar surface **304b** may be substantially the same as or smaller than that of the incision **104** (FIG. 1B) width B . Similarly, for example, the top planar surface **304a** having a width of W_2 may subsequently be inserted into incision **104** (FIG. 1B) having a width B , whereby the width of W_2 of the top planar surface **304a** may also be substantially the same as or smaller than that of the incision **104** (FIG. 1B) width B . If the incision provides, for example, access to the orbital floor **108** (FIG. 1B) of a patient, then the subsequently inserted top planar surface **304a** may be coupled to the already inserted bottom planar surface **304b** within the exposed orbital floor **108** region.

For providing a maximum expansion of the area corresponding to expandable surgical implant device **302**, the plurality of snap fit connectors **308a-308c** of the top planar surface **304a** may be coupled (e.g., snap fitted) to openings **310d-314d** of the bottom planar surface **304b**, respectively. For example, for an intermediate expansion of the area corresponding to expandable surgical implant device **302**, the plurality of snap fit connectors **308a-308c** of the top planar surface **304a** may be coupled (e.g., snap fitted) to either openings **310c-314c** or **310b-314b** of the bottom planar surface **304b**, respectively. A minimum expansion of the area corresponding to expandable surgical implant device **302** may be provided, whereby the plurality of snap fit connectors **308a-308c** of the top planar surface **304a** may alternatively be coupled (e.g., snap fitted) to openings **310a-314a** of the bottom planar surface **304b**, respectively.

The snap fit connectors **308a-308c** may include a flexible polyethylene material that enables it to deform when forcibly inserted into the respective openings of the snap fit receptacles **306a-306c**. Moreover, the top planar surface **304a** and the bottom planar surface **304b** may also include a thickness in the region of about 0.6-1.5 millimeters and each may have an embedded titanium mesh (not shown).

Referring to FIG. 3B, a modified exemplary embodiment of the expandable surgical implant device **302** is depicted. As illustrated, the top planar surface **304a** may include a top elongate raised portion **318a**, while the bottom planar surface **304b** may include a corresponding top channel region **320a** that receives the elongate raised portion **318a**. The top planar surface **304a** may also include a center elongate raised portion **318b**, while the bottom planar surface **304b** includes corresponding center channel region **320b** that receives the elongate raised portion **318b**. Finally, the top

planar surface **304a** may include a bottom elongate raised portion **318c**, while the bottom planar surface **304b** may include corresponding bottom channel region **320c** for receiving elongate raised portion **318c**.

In operation, the elongate raised portions **318a-318c** may snap fit into and slidably move within their respective channel regions **320a-320c**. The frictional forces between the coupled elongate raised portions **318a-318c** and their respective channel regions **320a-320c** may facilitate maintaining a positional relationship between both the top planar surface **304a** and the bottom planar surface **304b**. For example, referring to FIG. 3C, the combined expanded surface area of the expandable surgical implant device **302**, as governed by the non-overlapping portions of the top planar surface **304a** and the bottom planar surface **304b**, may be increased by sliding elongate raised portions **318a-318c** within their respective channel regions **320a-320c** from position PA (FIG. 3B) to position PB. Thus, the frictional forces between the coupled elongate raised portions **318a-318c** and their respective channel regions **320a-320c** may facilitate maintaining positional relationship PB between both the top planar surface **304a** and the bottom planar surface **304b**.

Referring to the plan view of FIG. 4A, another exemplary embodiment of an expandable surgical implant device **402** is depicted. As shown in expanded cross sectional view **403a**, the surgical implant device **402** may include a mating receptacle **404a** located on a vertical edge **406** of a first substantially planar portion **408a**. Also, surgical implant device **402** may include a mating connector **410a** located on a vertical edge **412** of a second substantially planar portion **408b**. The mating connector **410a** may snapably interlock with mating receptacle **404a**, thereby coupling the first and the second substantially planar portions **408a**, **408b** (FIG. 4B) at their respective vertical edges **406**, **412**.

Similarly, additional planar portions may be added to increase the surface area of the expandable implant device **402**. Thus, as shown in expanded cross sectional view **403b**, the surgical implant device **402** may include a mating receptacle **404b** located on a vertical edge **416** of a third substantially planar portion **408c**. Also, surgical implant device **402** may include a mating another mating connector **410b** located on the other vertical edge **414** of the second substantially planar portion **408b**. The mating connector **410b** may snapably interlock with mating receptacle **404b**, thereby coupling the second and the third substantially planar portions **408b**, **408c** (FIG. 4C) at their respective vertical edges **414**, **416**.

By providing the ability to couple the first substantially planar portion **408a**, the second substantially planar portion **408b**, and the third substantially planar portion **408c** in the described manner, each planar portion may be individually inserted into an incision of substantially the same width as either planar region, and subsequently coupled together within the region of the body receiving the expandable surgical implant device **402**. For example, the first substantially planar portion **408a** having a width of W_1 may be inserted into incision **104** (FIG. 1B) having a width B, whereby the width of W_1 of the first substantially planar portion **408a** may be substantially the same as or smaller than that of the incision **104** (FIG. 1B) width B. Similarly, for example, the second substantially planar portion **408b** having a width of W_2 may subsequently be inserted into incision **104** (FIG. 1B) having a width B, whereby the width of W_2 of the second substantially planar portion **408b** may also be substantially the same as or smaller than that of the incision **104** (FIG. 1B) width B. Also, for example, the third

substantially planar portion **408c** having a width of W_3 may subsequently be inserted into incision **104** (FIG. 1B) having a width B, whereby the width of W_3 of the third substantially planar portion **408c** may also be substantially the same as or smaller than that of the incision **104** (FIG. 1B) width B. If the incision provides, for example, access to the orbital floor **108** (FIG. 1B) of a patient, then the subsequently inserted second and third substantially planar portions **408b**, **408c** may be coupled to the already inserted first substantially planar portion **408a** within the exposed orbital floor **108** region.

The snap fitted mating connectors **410a**, **410b** and mating receptacles **404a**, **404b** may include a flexible polyethylene material that enables them to deform upon forced coupling. Moreover, the first, second, and third substantially planar portions **408a**, **408b**, **408c** may include a thickness in the region of about 0.6-1.5 millimeters and each may have an embedded titanium mesh (not shown).

It may be appreciated that the above non-limiting embodiments can be used in conjunction with any medical or other process (non-medical) involving incisions. The coupling and expanding mechanisms may also vary according to various use-parameters such as the location of the incision, size of the incision, and the surface area that the implant is required to cover. The thickness and types of materials also depend on the use (i.e., medical vs. non-medical). For example, in medical applications, the materials used in the formation of the implants should be bio-integratable and may, based on their use, have different thicknesses, flexibility, and strength.

The descriptions of the various embodiments of the present invention have been presented for purposes of illustration, but are not intended to be exhaustive or limited to the embodiments disclosed. Many modifications and variations will be apparent to those of ordinary skill in the art without departing from the scope and spirit of the described embodiments. The terminology used herein was chosen to best explain the principles of the one or more embodiments, the practical application or technical improvement over technologies found in the marketplace, or to enable others of ordinary skill in the art to understand the embodiments disclosed herein.

What is claimed is:

1. A surgical implant device adapted for repairing injury to the floor or walls of an orbit of an eye, comprising:
 - a first planar portion having a first top surface area;
 - a second planar portion having a second top surface area;
 - a swiveling mechanism that couples the first and the second planar portions for laterally swiveling the first and the second planar portions apart between an expanded state and an unexpanded state; and
 - an interlocking mechanism for maintaining the relative positions of the first and the second planar portions upon laterally swiveling laterally apart the first and the second planar portions to the expanded state, the interlocking mechanism including complementary interlocking structures located on the first and the second planar portions, wherein during the unexpanded state the surgical implant includes a top surface area, as observed from a plan view, corresponding to the first top surface area of the first planar portion, and wherein during the expanded state the surgical implant includes a top surface area, as observed from a plan view, corresponding to both the first top surface area of the first planar portion and at least a portion of the second top surface area of the second planar portion, in the unexpanded state the first and the second planar portions overlapping in a manner that, as observed from a

9

plan view, only the second planar portion is visible, and during the expanded state a first end region of the coupled first and second planar portions includes an increased width relative to a second end region of the coupled first and second planar portions opposing the first end region, the swiveling mechanism located adjacent the second end region having a smaller width relative to the first end region,

the surgical implant being adapted for placement within an incision in the unexpanded state and adapted to be laterally swiveled to the expanded state following placement within the incision, wherein in the expanded state, the surgical implant is adapted to cover an injury surface area located within the incision that includes a width dimension that is larger relative to a width dimension of the incision, the implant device as a whole having a planar shape adapted for placement within the incision.

2. The implant device of claim 1, wherein the first planar portion and the second planar portion comprise a thickness of about 0.6-1.5 millimeters.

3. A surgical implant device adapted for repairing injury to the floor or walls of an orbit of an eye, comprising:

a first planar portion having a first top surface area;

a second planar portion having a second top surface area;

a swiveling mechanism that couples the first and the second planar portions for laterally swiveling the first and the second planar portions apart between an expanded state and an unexpanded state; and

10

an interlocking mechanism for maintaining the relative positions of the first and the second planar portions upon laterally swiveling laterally apart the first and the second planar portions to the expanded state, wherein during the unexpanded state the surgical implant includes a top surface area, as observed from a plan view, corresponding to the first top surface area of the first planar portion, and wherein during the expanded state the surgical implant includes a top surface area, as observed from a plan view, corresponding to both the first top surface area of the first planar portion and at least a portion of the second top surface area of the second planar portion, in the unexpanded state the first and the second planar portions overlapping in a manner that, as observed from a plan view, only the second planar portion is visible, and during the expanded state a first end region of the coupled first and second planar portions includes an increased width relative to a second end region of the coupled first and second planar portions opposing the first end region, the swiveling mechanism located adjacent the second end region having a smaller width relative to the first end region, the implant device as a whole having a planar shape adapted for placement within the incision.

4. The implant device of claim 3, wherein the first planar portion and the second planar portion comprise a thickness of about 0.6-1.5 millimeters.

* * * * *